

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification: A61M 37/00, A61B 10/00	A2	(11) International Publication Number: WO 00/74763 (43) International Publication Date: 14 December 2000 (14.12.2000)
(21) International Application Number: PCT/US00/15312 (22) International Filing Date: 02 June 2000 (02.06.2000) (30) Priority Data: 09/448,107 23 November 1999 (23.11.1999) US 09/452,979 02 December 1999 (02.12.1999) US 09/453,109 02 December 1999 (02.12.1999) US 60/137,621 04 June 1999 (04.06.1999) US 60/146,200 29 July 1999 (29.07.1999) US (60) Parent Application or Grant GEORGIA TECH RESEARCH CORPORATION [/]; (). PRAUSNITZ, Mark, R. [/]; (). ALLEN, Mark, G. [/]; (). IENRY, Sebastien [/]; (). MCALLISTER, Devin, V. [/]; () . ACKLEY, Donald, F. [/]; (). GUJRAL, Jinder-Jeet [/]; (). JACKSON, Thomas [/]; (). PABST, Patrea, L. ; ().		Published

(54) Title: DEVICES AND METHODS FOR ENHANCED MICRONEEDLE PENETRATION OF BIOLOGICAL BARRIERS
 (54) Titre: DISPOSITIFS ET PROCÉDES PERMETTANT D'AMÉLIORER LA PÉNÉTRATION D'UNE MICROAIGUILLE À TRAVERS DES BARRIÈRES TISSULAIRES

(57) Abstract

Microneedle devices are provided for delivery of drugs across biological tissue and for controlled sampling of biological fluids in a minimally-invasive, painless, and convenient manner. The devices permit 1) drug delivery at clinically relevant rates across or into skin or other tissue barriers, and/or 2) *in vivo* sensing or withdrawal of biological fluids from the body, particularly from or through the skin or other tissue barriers. Drug delivery devices preferably include a plurality of hollow microneedles attached to or integrated into a substrate, and at least one reservoir (containing drug) selectively in communication with the microneedles, wherein the amount of drug to be delivered can be selectively altered. Withdrawal or sensing microneedle devices preferably include microneedles attached to or integrated into a substrate, and at least one collection chamber and or sensor in communication with the microneedles. Preferred embodiments further include a means for inducing biological fluid, such as interstitial fluid, to be drawn through the microneedles and into the collection chamber for analysis. Also provided are microneedle devices and methods for the enhanced transport of molecules across tissue by improving the interaction of an array of microneedles and a deformable, elastic biological barrier, such as human skin. The devices and methods act to 1) limit the elasticity, 2) adapt to the elasticity, 3) utilize alternate ways of creating the holes for the microneedles to penetrate the biological barrier, other than the simply direct pressure of the microneedle substrate to the barrier surface, or 4) combination of 1)-3).

(57) Abrégé

L'invention concerne des dispositifs à microaiguilles, permettant de distribuer des médicaments à travers un tissu biologique, et de réguler un échantillonnage de fluides corporels de manière appropriée et peu invasive, sans causer de douleur. Ces dispositifs permettent 1) de distribuer un médicament à travers de la peau ou d'autres barrières tissulaires, ou dans celles-ci, à des vitesses cliniquement acceptables, et/ou 2) à détecter *in vivo* ou à évacuer des fluides biologiques du corps, en particulier à partir de la peau ou d'autres barrières tissulaires, ou à travers celles-ci. Les dispositifs de distribution de médicaments comprennent, de préférence, une pluralité de microaiguilles creuses fixées à un substrat ou incorporés dans celui-ci, et au moins un réservoir (contenant un médicament) en communication fluide sélective avec lesdites microaiguilles, dans lesquelles la quantité de médicament à distribuer est sélectivement modifiée. Les dispositifs de détection ou d'évacuation à microaiguilles comprennent des microaiguilles fixées à un substrat ou incorporés dans celui-ci, et au moins une chambre de collecte et/ou un capteur en communication fluide avec lesdites microaiguilles. Des modes de réalisation préférés comprennent également un organe permettant d'aspirer un fluide biologique, tel qu'un fluide interstitiel, dans les microaiguilles et dans la chambre de collecte pour analyse. L'invention concerne également des dispositifs à microaiguilles et des procédés permettant d'améliorer le transport des molécules à travers un tissu, au moyen d'une meilleure interaction entre un réseau de microaiguilles et une barrière biologique, élastique, déformable, telle que la peau humaine. Ces dispositifs et ces procédés agissent de façon 1) à limiter l'élasticité de la peau, 2) à s'adapter à cette élasticité, 3) à utiliser des manières alternatives autres que la simple pression directe du substrat de microaiguille sur la surface de la barrière, afin de produire des trous permettant la pénétration des microaiguilles dans la barrière biologique, ou 4) à utiliser une combinaison des étapes 1) et 3).

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
14 December 2000 (14.12.2000)

PCT

(10) International Publication Number
WO 00/74763 A2

(51) International Patent Classification⁷: A61M 37/00,
A61B 10/00

(21) International Application Number: PCT/US00/15312

(22) International Filing Date: 2 June 2000 (02.06.2000)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/137,621 4 June 1999 (04.06.1999) US
60/146,200 29 July 1999 (29.07.1999) US
09/448,107 23 November 1999 (23.11.1999) US
09/452,979 2 December 1999 (02.12.1999) US
09/453,109 2 December 1999 (02.12.1999) US

(71) Applicant: GEORGIA TECH RESEARCH CORPORATION [US/US]; 400 Tenth Street, Centennial Research Building, Atlanta, GA 30332-0414 (US).

(72) Inventors: PRAUSNITZ, Mark, R.; 417 West Howard Avenue, Decatur, GA 30030 (US). ALLEN, Mark, G.; 425 Spalding Drive, Atlanta, GA 30328 (US). HENRY,

Sebastien; 1511 Vinings Parkway, Smyrna, GA 30080 (US). MCALLISTER, Devin, V.; 49 Geddes Street, Holley, NY 14470 (US). ACKLEY, Donald, E.; 2033 Cambridge Avenue, Cardiff, CA 92007 (US). GUJRAL, Inder-Jeet; 111-9 Trowbridge Street, Cambridge, MA 02138 (US). JACKSON, Thomas; 7135 Olivetas Avenue, La Jolla, CA 92037 (US).


(74) Agents: PABST, Patrea, L. et al.; Arnall Golden & Gregory, LLP, 2800 One Atlantic Center, 1201 West Peachtree Street, Atlanta, GA 30309-3450 (US).

(81) Designated States (*national*): AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, DE, DK, DM, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, UZ, VN, YU, ZA, ZW.

(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: DEVICES AND METHODS FOR ENHANCED MICRONEEDLE PENETRATION OF BIOLOGICAL BARRIERS

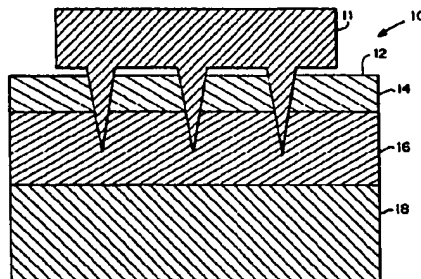

WO 00/74763 A2 (57) Abstract: Microneedle devices are provided for delivery of drugs across biological tissue and for controlled sampling of biological fluids in a minimally-invasive, painless, and convenient manner. The devices permit 1) drug delivery at clinically relevant rates across or into skin or other tissue barriers, and/or 2) *in vivo* sensing or withdrawal of biological fluids from the body, particularly from or through the skin or other tissue barriers. Drug delivery devices preferably include a plurality of hollow microneedles attached to or integrated into a substrate, and at least one reservoir (containing drug) selectively in communication with the microneedles, wherein the amount of drug to be delivered can be selectively altered. Withdrawal or sensing microneedle devices preferably include microneedles attached to or integrated into a substrate, and at least one collection chamber and or sensor in communication with the microneedles. Preferred embodiments further include a means for inducing biological fluid, such as interstitial fluid, to be drawn through the microneedles and into the collection chamber for analysis. Also provided are microneedle devices and methods for the enhanced transport of molecules across tissue by improving the interaction of an array of microneedles and a deformable, elastic biological barrier, such as human skin. The devices and methods act to 1) limit the elasticity, 2) adapt to the elasticity, 3) utilize alternate ways of creating the holes for the microneedles to penetrate the biological barrier, other than the simply direct pressure of the microneedle substrate to the barrier surface, or 4) combination of 1)-3).

1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20 21 22 23 24 25 26 27 28 29 30 31 32 33 34 35 36 37 38 39 40 41 42 43 44 45 46 47 48 49 50 51 52

— Without international search report and to be republished upon receipt of that report.

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Description

5

10

15

20

25

30

35

40

45

50

55

5

DEVICES AND METHODS FOR ENHANCED MICRONEEDLE PENETRATION OF BIOLOGICAL BARRIERS

10

Background Of The Invention

5 This invention is generally in the field of devices for the transport of therapeutic or biological molecules across tissue barriers, such as for drug delivery or for the withdrawal and sensing of biological fluids, such as in the analysis of blood glucose levels.

15

10 A frequent limitation of drugs and therapeutic agents is their delivery: how to transport drugs across biological barriers in the body (e.g., the skin, the oral mucosa, the blood-brain barrier), which normally do not transport drugs at rates that are therapeutically useful or optimal.

20

Drugs commonly are administered orally as pills or capsules. Many drugs, however, cannot be effectively delivered in this manner, due to degradation in the gastrointestinal tract and/or elimination by the liver. Moreover, some drugs cannot effectively diffuse across the intestinal mucosa. Patient compliance may also be a problem in therapies requiring, for example, that pills be taken at particular intervals over a prolonged time.

25

30 Another common technique for delivering drugs across a biological barrier is the use of a needle, such as those used with standard syringes or catheters, to transport drugs across (through) the skin. While effective for this purpose, needles generally cause pain; local damage to the skin at the site of insertion; bleeding, which increases the risk of disease transmission; and a wound sufficiently large to be a site of infection. Needle techniques also generally require administration by one trained in its use, and are not preferred for frequent routine use due to the vascular damage caused by repeated punctures, nor are they desirable for long term controlled continuous drug delivery.

30

35

25 Similarly, current methods of sampling biological fluids are invasive and suffer from the same disadvantages. For example, the extraction of analytes through the skin is critical to diabetic patients, who typically must measure blood glucose several times per day in order to optimize insulin treatment and thereby reduce the severe long-term complications of the disease. Currently, diabetics do this by pricking the highly vascularized fingertips with a lancet to perforate the skin, then

40

45

50

55

5 milking the skin with manual pressure to produce a drop of blood, which is then
assayed for glucose using a disposable diagnostic strip and a meter into which the
strip fits. This method of glucose measurement has the major disadvantage that it is
10 painful, so diabetics do not like to obtain a glucose measurement as often as is
5 medically indicated. It would therefore be highly useful to be able to obtain a
sample of blood, lymph, or interstitial fluid more quickly, using an easier procedure,
and relatively noninvasively. It also would be advantageous to be able to repeatedly
15 or continually extract analyte transdermally over a period of time.

An alternative delivery technique is the transdermal patch, which usually
10 relies on diffusion of the drug across the skin. However, this method is not useful
for many drugs, due to the poor permeability (i.e. effective barrier properties) of the
20 skin. The rate of diffusion depends in part on the size and hydrophilicity of the drug
molecules and the concentration gradient across the stratum corneum. Few drugs
have the necessary physiochemical properties to be effectively delivered through the
25 skin by passive diffusion. Iontophoresis, electroporation, ultrasound, and heat (so-
called active systems) have been used in an attempt to improve the rate of delivery.
While providing varying degrees of enhancement, these techniques are not suitable
for all types of drugs, failing to provide the desired level of delivery. In some cases,
30 they are also painful and inconvenient or impractical for continuous controlled drug
20 delivery over a period of hours or days. Some proposed alternatives to the needle
require the use of (1) lasers or heat to create a hole in the skin, which is
inconvenient, expensive, or undesirable for repeated use; (2) electric fields or
35 ultrasound, which also is inconvenient and expensive; or (3) chemical or biological
penetration enhancing agents, which can be irritating to the tissue and undesirable
25 for repeated use. Attempts have been made to design alternative devices for active
transfer of drugs, or analyte to be measured, through the skin.

40 For example, U.S. Patent No. 5,879,326 to Godshall et al. and PCT WO
96/37256 by Silicon Microdevices, Inc. disclose a transdermal drug delivery
apparatus that includes a cutter portion having a plurality of microprotrusions, which
45 have straight sidewalls, extending from a substrate that is in communication with a
30 drug reservoir. In operation, the microprotrusions penetrate the skin until limited by
a stop region of the substrate and then are moved parallel to the skin to create
incisions. Channels in the substrate adjacent to the microprotrusions allow drug
50

5 from the reservoir to flow to the skin near the area disrupted by the
microprotrusions. Merely creating a wound, rather than using a needle which
conveys drug through an enclosed channel into the site of administration, creates
10 variability in dosage.

5 U.S. Patent No. 5,250,023 to Lee *et al.* discloses a transdermal drug delivery
device, which includes a plurality of needles having a diameter in the range of 50 to
400 μm . The needles are supported in a water-swellable polymer substrate through
15 which a drug solution permeates to contact the surface of the skin. An electric
current is applied to the device to open the pathways created by the needles.
10 following their withdrawal from the skin upon swelling of the polymer substrate.

20 PCT WO 93/17754 by Gross *et al.* discloses another transdermal drug
delivery device that includes a housing having a liquid drug reservoir and a plurality
of tubular elements for transporting liquid drug into the skin. The tubular elements
may be in the form of hollow needles having *inner* diameters of less than 1 mm and
25 an outer diameter of 1.0 mm.

While each of these devices has potential use, there remains a need for better
drug delivery devices, which make smaller incisions, deliver drug with greater
efficiency (greater drug delivery per quantity applied) and less variability of drug
30 administration, and/or are easier to use. In view of these needs, microneedle devices
20 have been developed, which are described in PCT WO 99/64580. Certain
embodiments of the device were found to readily penetrate skin samples in *in vitro*
experiments, but not always provide uniform or complete insertion of the microneedles
35 into some areas of the skin *in vivo*, as the stratum corneum and underlying tissues are
highly deformable and elastic over much of the body.

25 It is therefore an object of the present invention to provide a microneedle
device for relatively painless, controlled, safe, convenient transdermal delivery of
40 drugs.

It is a further object of the present invention to provide a microneedle device
controlled sampling or sensing of biological fluids in a minimally-invasive, painless,
45 and convenient manner.
30

It is another object of the present invention to provide methods and devices
for improving the control of microneedle insertion into the body of a patient.

5

Summary Of The Invention

10

Microneedle devices are provided for delivery of drugs across or into biological tissue and for controlled sampling of biological fluids in a minimally-invasive, painless, and convenient manner. The microneedle devices permit (1) drug delivery at clinically relevant rates across or into skin or other tissue barriers, and (2) *in vivo* sensing or withdrawal of biological fluids from the body, particularly from or through the skin or other tissue barriers.

15

20

In a preferred embodiment for drug delivery, the devices include a plurality of hollow microneedles, which are attached to or integrated into a substrate, and at least one reservoir selectably in communication with the microneedles, wherein the volume or amount of drug to be delivered can be selectively altered. The reservoir contains the drug to be delivered, and can be formed of a deformable, preferably elastic, material. The device also can include means for compressing the reservoir to drive the drug from the reservoir through the microneedles. The means can include a plunger or osmotic pump. In one embodiment, the reservoir is a syringe or pump connected to the substrate. The device also can include a sealing mechanism to contain the drug in one or more of the reservoirs until it is ready to be delivered or mixed with a liquid carrier. In one embodiment, the sealing mechanism is a fracturable barrier interposed between the reservoir and the substrate. The device also can include a means for providing feedback, such as color change, to the user to indicate that delivery has been initiated and/or completed. In another embodiment, the microneedle device further includes a rate control means, such as a semi-permeable membrane, to regulate the rate or extent of drug which flows through the microneedles.

25

30

35

In a preferred embodiment for withdrawal or sensing, the microneedle device includes one or more microneedles, preferably in a three-dimensional array, a substrate to which the microneedles are connected, and at least one collection chamber and/or sensor in communication with the microneedles. Preferred embodiments further include a means for inducing biological fluid, such as blood, lymph, or interstitial fluid, to be drawn through the microneedles and into the collection chamber for analysis. This induction preferably is accomplished by use of a pressure gradient, which can be created for example by selectively increasing the interior volume of the collection chamber, which includes an elastic or movable

40

45

50

55

5 portion engaged to a rigid base. In a preferred embodiment, the microneedle device further comprises means for transduction, storage, transmission, and display of measured values. The microneedle device also preferably includes means for
10 securing the device to a biological barrier during withdrawal or sensing.

5 The microneedle devices preferably are provided with means for preventing undesired reuse of or contact with the microneedles. These means can include protective packaging, such as a peelable liner that temporarily covers the tips of the
15 microneedles. The packaging also can be used to shear off the microneedles following their intended use, thereby preventing their reuse.

10 Also provided are microneedle devices and methods of use thereof for the enhanced transport of molecules, including drugs and biological molecules, across tissue by improving the interaction of an array of microneedles and a deformable, elastic biological barrier, such as human skin. The devices and methods act to (1) limit the elasticity, (2) adapt to the elasticity, (3) utilize alternate ways of creating
20 the holes for the microneedles to penetrate the biological barrier, other than the simply direct pressure of the microneedle substrate to the barrier surface, or (4) combinations of (1)-(3).

30 In preferred embodiments for limiting the elasticity of skin, the microneedle device includes features suitable for stretching, pulling, or pinching the skin to present a more rigid, less deformable, surface in the area to which the microneedles are applied (i.e. penetrate). For example, a vacuum can be applied to the area of the skin at the site of microneedle application to pull it taut and/or pull the skin onto the tips of the microneedles. Alternatively or in addition, the elasticity of skin can be reduced by applying a thin film or membrane over the skin surface at the site of
35 application, so as to keep the skin tight, limiting the ability of the skin to stretch at the application site. The microneedles are then pushed through the film or membrane and into the skin.

40 In preferred embodiments for adapting the device to the elasticity of skin, the microneedles of the device include individual extensions or are provided in a curved three dimensional array, for example, by using a flexible substrate and/or varying
45 the height of the microneedles in the array. In another embodiment, the microneedles are applied to the skin surface at an increased velocity, thereby

5 reducing the time available for the stratum comeum and underlying tissues to deform from contact with the tips or entire length of the microneedles.

10 In a preferred embodiment for creating holes in the skin for microneedles, tiny holes are burned into the skin, for example, by heating of the tips of the
5 microneedles and/or by using a laser. In another embodiment, a focused blast of high pressure gas is used to create the holes.

Brief Description Of The Drawings

15 Figures 1a-e are side cross-sectional views of a method for making hollow microneedles.

10 Figures 2a-g are side cross-sectional views of a method for making a hollow microneedle.

20 Figures 3a-d are side cross-sectional views illustrating a preferred method for making hollow microneedles.

Figures 4a-d are side cross-sectional views illustrating a preferred method for
25 making hollow silicon microtubes.

Figures 5a-e are side cross-sectional views illustrating a preferred method for making hollow metal microtubes.

Figures 6a-d are side cross-sectional views illustrating a preferred method for
30 making tapered metal microneedles.

20 Figures 7a-d are side cross-sectional views illustrating a method for making tapered microneedles using laser-formed molds.

Figures 8a-f are side cross-sectional views illustrating a second method for
35 making tapered microneedles using laser-formed molds.

Figure 9 is a side elevational view of a schematic of an embodiment of the
25 microneedle device inserted into undeformed skin.

Figures 10a-d are illustrations of microneedle devices having various
40 embodiments of microneedle extensions.

Figures 11a-c are cross-sectional views illustrating microneedle devices
45 having curved substrates (11a), varying microneedle height (11b), and linear
30 microneedle arrays (11c).

Figures 12a-c are cross-sectional views illustrating preferred microneedle
devices inserted into skin with altered elasticity.

5 Figures 13a-c are cross-sectional views illustrating preferred embodiments of microneedle devices which can apply suction to skin at the site of insertion.

10 Figures 14a-c are cross-sectional (14a-b) and perspective (14c) views illustrating preferred embodiments of microneedle devices which stretch the skin at the site of insertion.

15 Figures 15a-c are cross-sectional views illustrating examples of microneedle devices which pinch the skin at the site of insertion.

 Figure 16 is a cross-sectional view of a preferred embodiment of a microneedle device for use in localized heating of skin.

20 Figure 17 is a cross-sectional view of a preferred embodiment of a microneedle device having a microneedle reinforcing layer.

25 Figures 18a-b are cross-sectional views of a preferred embodiment of a microneedle device having a flexible substrate in an unactivated position (18a) and an activated position (18b).

 Figure 19 is a cross-sectional view a preferred embodiment of a microneedle device having arrays of microneedles with spaces between the arrays.

30 Figures 20a-c are cross-sectional views of preferred embodiments of a microneedle drug delivery device. The device of Figure 20a includes a reservoir and is suitable for transdermal drug delivery. The device of Figures 20a and 20b includes a deformable reservoir, wherein delivery is activated by manual, e.g., finger or thumb, pressure applied to compress the reservoir directly (20b) or indirectly (20c).

35 Figure 21 is a cross-sectional view of another preferred embodiment of a microneedle drug delivery device, wherein delivery is activated by manual pressure applied via a plunger to compress the reservoir.

40 Figure 22 is a cross-sectional view of another preferred embodiment of a microneedle drug delivery device, wherein delivery is activated by releasing a compressed spring which forces the plunger to compress the reservoir.

45 Figures 23a-b are cross-sectional views of preferred embodiments of a microneedle drug delivery device having a multiple chambered reservoirs.

50 Figure 24 is a cross-sectional view of a preferred embodiment of the microneedle drug delivery device, which incorporates an osmotic pump to force the drug contents from the reservoir.

5 Figure 25 is a cross-sectional view of a preferred embodiment of a microneedle device for fluid withdrawal.

10 Figure 26 is a cross-sectional view of another preferred embodiment of a microneedle device for fluid withdrawal.

5 Figures 27a-c are cross-sectional views of preferred embodiments of a microneedle device in which a sensor is included on the external surface of a hollow needle (27a), on the internal bore surface of a hollow needle (27b), and within the
15 pores of a porous, hollow needle (27c).

Detailed Description Of The Invention

10 1. Biological Barriers

20 The devices disclosed herein are useful in transport of material into or across biological barriers including the skin (or parts thereof); the blood-brain barrier; mucosal tissue (e.g., oral, nasal, ocular, vaginal, urethral, gastrointestinal, respiratory); blood vessels; lymphatic vessels; or cell membranes (e.g., for the
25 introduction of material into the interior of a cell or cells). The biological barriers can be in humans or other types of animals, as well as in plants, insects, or other organisms, including bacteria, yeast, fungi, and embryos. The microneedle devices can be applied to tissue internally with the aid of a catheter or laparoscope. For
30 certain applications, such as for drug delivery to an internal tissue, the devices can be surgically implanted.

35 In a preferred embodiment, the microneedle device disclosed herein is applied to skin. The stratum corneum is the outer layer, generally between 10 and 50 cells, or between 10 and 20 μm thick. Unlike other tissue in the body, the stratum corneum contains "cells" (called keratinocytes) filled with bundles of cross-
40 linked keratin and keratohyalin surrounded by an extracellular matrix of lipids. It is this structure that is believed to give skin its barrier properties, which prevents therapeutic transdermal administration of many drugs. Below the stratum corneum is the viable epidermis, which is between 50 and 100 μm thick. The viable
45 epidermis contains no blood vessels, and it exchanges metabolites by diffusion to and from the dermis. Beneath the viable epidermis is the dermis, which is between 1 and 3 mm thick and contains blood vessels, lymphatics, and nerves.

As used herein, references to using the microneedle devices on "skin" also include using the microneedle devices with other biological barriers unless expressly limited to only skin.

2. The Microneedle Device

The microneedle devices disclosed herein include a substrate, one or more microneedles, and optionally (i) a reservoir for delivery of drugs, (ii) a fluid collection chamber for collection of biological fluid, and/or (iii) a sensor for sensing an analyte, all or any of which (i-iii) can be selectably in communication with at least one microneedle. The devices also can include one or more pumps, sensors, and/or microprocessors to control the interaction of the foregoing. The microneedle device preferably includes penetration enhancing features to alter or adapt to deformable and elastic biological barriers, such as the skin over much of the human body. Preferably, the microneedles are provided as a multi-dimensional array, in contrast to a device with a single microneedle or single row of microneedles. The microneedle device can be adapted to be a single-use, disposable device, or can be adapted to be fully or partially reusable.

In one embodiment for delivery of drugs, the microneedle device includes at least three components: a plurality of microneedles; a substrate to which the base of the microneedles are secured or integrated; and at least one reservoir that is selectably in fluid connection with one or more of the microneedles.

a. Substrate

The substrate of the device can be constructed from a variety of materials, including metals, ceramics, semiconductors, organics, polymers, and composites. The substrate includes the base to which the microneedles are attached or integrally formed. A reservoir and/or fluid collection chamber also may be attached to, or integrally formed with, the substrate. The substrate can be adapted to fit a Luer-Lock syringe or other conventionally used drug delivery or fluid withdrawal device that currently uses hypodermic needles as the barrier penetration method. A fluid collection chamber and/or sensor can be attached to the substrate or formed (e.g., as part of the substrate) to communicate directly with the base of the microneedles.

In one embodiment of the device, the substrate is formed from a thin, rigid material that is sufficiently stiff so as to force the attached microneedles through the

biological barrier in such areas where the barrier resists deformation by the microneedles.

In a preferred embodiment of the device, the substrate, and possibly other components, is formed from flexible materials, or have appropriate materials so as to be flexible, to allow the device to fit the contours of the biological barrier (such as the skin, vessel walls, or the eye) to which the device is applied and to adapt to barrier deformations that may occur when the microneedle device is applied. A flexible device further facilitates more consistent penetration during use, since penetration can be limited by deviations in the attachment surface. For example, the surface of human skin is not flat due to dermatoglyphics, i.e. tiny wrinkles, and hair, and is highly deformable. The flexible substrate can be deformed mechanically (for example, using an actuator or simply by fluid pressure) in order to pierce the biological barrier. Conformality of the flexible device to the skin can be further enhanced by using an external force, such as a uniform pressure, to aid insertion of the microneedles into the biological barrier. However, for some biological barriers or applications, a rigid substrate may be preferred.

b. Microneedle

The microneedles of the device can be constructed from a variety of materials, including metals, ceramics, semiconductors, organics, polymers, and composites. Representative materials of construction include pharmaceutical grade stainless steel, gold, titanium, nickel, iron, gold, tin, chromium, copper, palladium, platinum, alloys of these or other metals, silicon, silicon dioxide, and polymers. Representative biodegradable polymers include polymers of hydroxy acids such as lactic acid and glycolic acid polylactide, polyglycolide, polylactide-co-glycolide, and copolymers with PEG, polyanhydrides, poly(ortho)esters, polyurethanes, poly(butyric acid), poly(valeric acid), and poly(lactide-co-caprolactone). Representative non-biodegradable polymers include polycarbonate, polymethacrylic acid, ethylenevinyl acetate, polytetrafluoroethylene (TEFLONTM), and polyesters.

Generally, the microneedles should have the mechanical strength to remain intact for delivery of drugs, or serve as a conduit for the collection of biological fluid, while being inserted into the skin, while remaining in place for up to a number of days, and while being removed. In embodiments where the microneedles are formed of biodegradable polymers, however, this mechanical requirement is less

5 stringent, since the microneedles or tips thereof can break off, for example in the
skin, and will biodegrade. Nonetheless, even a biodegradable microneedle still
needs to remain intact at least long enough for the microneedle to serve its intended
10 purpose (e.g., its conduit function). Therefore, biodegradable microneedles can
5 provide an increased level of safety, as compared to nonbiodegradable ones. The
microneedles generally should be sterilizable using standard methods such as
ethylene oxide or gamma irradiation.

15 The microneedles can be formed of a nonporous solid, a porous solid (with
or without a sealed coating or exterior portion), or hollow. As used herein, the term
10 "porous" means having pores or voids throughout at least a portion of the
microneedle structure, sufficiently large and sufficiently interconnected to permit
20 passage of fluid and/or solid materials through the microneedle. As used herein, the
term "hollow" means having one or more substantially annular bores or channels
through the interior of the microneedle structure, having a diameter sufficiently large
25 to permit passage of fluid and/or solid materials through the microneedle. The
annular bores may extend throughout all or a portion of the needle in the direction of
the tip to the base, extending parallel to the direction of the needle or branching or
exiting at a side of the needle, as appropriate. A solid or porous microneedle can be
30 hollow. One of skill in the art can select the appropriate porosity and/or bore
20 features required for specific applications. For example, one can adjust the pore size
or bore diameter to permit passage of the particular material to be transported
through the microneedle device. The inner surface of the bore of hollow
35 microneedles can be made rough to enhance cell membrane disruption for those
applications in which cell disruption is useful.

25 The microneedles can have straight or tapered shafts. A hollow microneedle
that has a substantially uniform diameter, which needle does not taper to a point, is
40 referred to herein as a "microtube." As used herein, the term "microneedle"
includes both microtubes and tapered needles unless otherwise indicated. In one
embodiment, the diameter of the microneedle is greatest at the base end of the
45 microneedle and tapers to a point at the end distal the base. The microneedle can
also be fabricated to have a shaft that includes both a straight (untapered) portion
and a tapered portion.

5 In a preferred embodiment for drug delivery, the microneedles are hollow: that is, each contains at least one substantially annular bore or channel having a diameter large enough to permit passage of a drug-containing fluid and/or solid materials through the microneedle. The bores may be linear, i.e. extend upwardly
10 from needle base to needle tip, or they may take a more complex path, e.g. extend upwardly from the needle base, but then lead to one or more 'portholes' or 'slits' on the sides of the needles, rather than an opening at the needle tip.

15 The microneedles can be formed with shafts that have a circular cross-section in the perpendicular, or the cross-section can be non-circular. For example, the cross-section of the microneedle can be polygonal (e.g. star-shaped, square, triangular), oblong, or another shape. The shaft can have one or more bores. The cross-sectional dimensions typically are between about 10 nm and 1 mm, preferably between 1 and 500 μm , and more preferably between 10 and 200 μm . The outer diameter is typically between about 10 μm and about 100 μm , and the inner
20 diameter is typically between about 3 μm and about 80 μm .

The length of the microneedles typically is between about 10 μm and 1 mm, preferably between 100 and 1 mm, more preferably between 100 and 500 μm , and more preferably between 150 and 350 μm . An array of microneedles can include a mixture of microneedles having, for example, various lengths, outer diameters, inner
25 diameters, cross-sectional shapes, and spacing between the microneedles. Preferably, the microneedles are sized to avoid or minimize contact with nerve endings in the biological tissue, such as the dermis, thereby eliminating or reducing pain when the microneedles are inserted, for example into the skin.

The microneedles can be oriented perpendicular or at an angle to the substrate. Preferably, the microneedles are oriented perpendicular to the substrate to provide structural strength and to permit ease of insertion into the tissue. An array of microneedles can include a mixture of microneedle orientations, heights, spacings, or other parameters. This variation in an array can be useful, for example, if different microneedles are to provide different sensing or insertion functions.

30 In embodiments for sensing and/or withdrawal, the microneedles function as a conduit, a sensing element, or a combination thereof. In one embodiment, one or more of the microneedles are coated (if solid, porous, or hollow) and/or at least

5 partially filled (if porous or hollow) with a sensing or diffusion-modifying material.
In one embodiment, the microneedle can have one or more holes (ports) or slits
10 positioned on the sides of the shaft of a hollow microneedle having a blunt, open, or
closed tip. This design may reduce blockage of the conduit, for example, due to
5 tissue or cells when the microneedles are inserted.

c. Reservoir

15 In some embodiments, particularly those for drug delivery and fluid
extraction, the microneedle device includes a reservoir in communication, preferably
selectably so, with the microneedles. The reservoir can be attached to the substrate
10 by any suitable means. In a preferred embodiment, the reservoir is attached to the
back of the substrate (opposite the microneedles) around the periphery, using an
20 adhesive agent (e.g., glue). A gasket may also be used to facilitate formation of a
fluid-tight seal.

In a preferred embodiment, the reservoir contains drug, for delivery through
25 the microneedles. The reservoir may be a hollow vessel, a porous matrix, or a solid
form including drug which is transported therefrom. The reservoir can be formed
from a variety of materials that are compatible with the drug or biological fluid
30 contained therein. Preferred materials include natural and synthetic polymers,
metals, ceramics, semiconductors, organics, and composites. In one embodiment,
20 the reservoir is a standard syringe.

The microneedle device can include one or a plurality of chambers for
35 storing materials to be delivered. In the embodiment having multiple chambers,
each can be in fluid connection with all or a portion of the microneedles of the
device array. In one embodiment, at least two chambers are used to separately
25 contain drug (e.g., a lyophilized drug, such as a vaccine) and an administration
vehicle (e.g., saline) in order to prevent or minimize degradation during storage.
40 Immediately before use, the contents of the chambers are mixed. Mixing can be
triggered by any means, including, for example, mechanical disruption (i.e.
puncturing or breaking), changing the porosity, or electrochemical degradation of
45 the walls or membranes separating the chambers. In another embodiment, a single
30 device is used to deliver different drugs, which are stored separately in different
chambers. In this embodiment, the rate of delivery of each drug can be
50 independently controlled.

5 In a preferred embodiment, the reservoir should be in direct contact with the microneedles and have holes through which drug could exit the reservoir and flow into the interior of hollow or porous microneedles. In another preferred
10 embodiment, the reservoir has holes which permit the drug to transport out of the reservoir and onto the skin surface. From there, drug is transported into the skin, either through hollow or porous microneedles, along the sides of solid microneedles, or through pathways created by microneedles in the skin.

15 In a preferred embodiment for drug delivery, the reservoir is selectively in connection with the microneedle bore, such that the reservoir contents can flow from the reservoir and out through the microneedle tip, into the target tissue. Typically, it is attached to, or integrated into, the substrate, either integrally (as in a one-piece device) or at the moment of drug delivery (as with a Luer-lock type device). The reservoir is to provide suitable, leak-free storage of the drug composition before it is to be delivered. The reservoir should keep the drug composition free of
20 contaminants and degradation-enhancing agents. For example, the reservoir should exclude light when the drug composition contains photo-sensitive materials, and should include an oxygen barrier material in order to minimize exposure of drugs sensitive to oxidation. Also, the reservoir should keep volatile materials inside the reservoir, for example, to prevent water from evaporating, causing the drug
25 composition to dry out and become undeliverable.

The drug reservoir can be substantially rigid or readily deformable. The reservoir can be formed from one or more polymers, metals, ceramics, or combinations thereof. In a preferred embodiment, the reservoir includes a volume surrounded by one or more walls, or includes a porous material, such as a sponge,
30 which can retain, for example, the drug liquid until the material is compressed.

35 In a preferred embodiment, the reservoir is formed of an elastic material, such as an elastomeric polymer or rubber. For example, the reservoir can be a balloon-like pouch that is stretched (in tension) when filled with a fluid drug composition to be delivered.

40 The reservoir of a single microneedle device can include a plurality of compartments that are isolated from one another and/or from a portion of the microneedles in an array. The device can, for example, be provided to deliver different drugs through different needles, or to deliver the same or different drugs at
45

5 different rates or at different times (Figure 23a). Alternatively, the contents of the
different compartments can be combined with one another, for example, by piercing,
or otherwise removing, a barrier between the compartments, so as to allow the
10 materials to mix. In a preferred embodiment, one compartment contains a saline
5 solution or another delivery vehicle, while another compartment contains
lyophilized drug (Figure 23b). In a preferred embodiment, the reservoir is a
standard or Luer-Lock syringe adapted to connect to a microneedle array.

15 d. Collection Chamber

In embodiments for extraction, the device preferably includes a fluid
10 collection chamber. The fluid collection chamber is selectably in connection with
the microneedle bores or pores, such that a biological fluid can flow from the tissue
20 surrounding the microneedle, through the microneedle, and into the collection
chamber. Typically, the collection chamber is attached to, or integrated into, the
substrate. The chamber should function to contain a biological fluid sample so as to
25 permit analysis within the microneedle device or following transfer to a separate
analytical device.

The collection chamber can be substantially rigid or readily deformable. The
collection chamber can be formed from one or more polymers, metals, ceramics,
30 semiconductor, or combinations thereof. In a preferred embodiment, the collection
20 chamber contains a porous or absorbent material, such as a sponge, gel, or paper or
polymeric strip. The material can be permanently contained or removable, and can
function as a diagnostic element or substrate for use in analytical devices. The
35 chamber can initially be empty or can contain a gas or one or more reagents in any
form (e.g., liquid or solid particles). In one embodiment, at least a portion of the
25 interior walls of the chamber are coated with a reagent for assaying the biological
fluid.

40 In a preferred embodiment, the collection chamber is formed of an elastic
material, such as an elastomeric polymer or rubber. For example, the collection
chamber can be a collapsed balloon-like pouch that expands when the biological
45 30 fluid is drawn into the collection chamber.

The collection chamber of a microneedle device can include a plurality of
compartments that are temporarily or permanently isolated from one another and/or
50 from a portion of the microneedles in an array. The device can, for example, be

5 provided to collect or sense through different needles at different rates or at different
times into the different compartments. Alternatively, some of the different
compartments can contain analytical reagents which can be combined with the
10 biological fluid sample, for example, by piercing, or otherwise removing, a barrier
5 between the compartments, so as to allow the materials to mix for analysis.

In another preferred embodiment, the collection chamber is adapted to
receive and use standard glucose sensing strips, which can be loaded into the
15 microneedle device before, during, or after the biological fluid is extracted.

Two embodiments of the microneedle device are shown in Figures 25-26. In
10 Figure 25, microneedle device 610 includes substrate 612 from which a three-
dimensional array of microneedles 614 protrude. As shown, the annular bore of the
microneedles 614 extends through the substrate 612. The device 610 also includes
20 fluid collection chamber 616 which is in fluid connection with the microneedles 614.
Fluid collection chamber 616 includes an access port 618 through which collected
25 fluid can be withdrawn from collection chamber 616, and/or through which a
withdrawing force, such as a vacuum, can be applied. In Figure 26, microneedle
device 620 includes substrate 612 from which a three-dimensional array of
microneedles 614 protrude, and fluid collection chamber 616, as well as elastic cap
30 622 and one-way valve 624. The interior of elastic cap 622 is in communication
20 with, or open to, fluid collection chamber 616.

e. Transport Control Components

The microneedle device also must be capable of transporting material across
35 the barrier at a useful rate. For example, the microneedle device must be capable of
delivering drug across the skin at a rate sufficient to be therapeutically useful. The
25 device may include a housing with microelectronics and other micromachined
structures to control the rate of delivery either according to a preprogrammed
40 schedule or through active interface with the patient, a healthcare professional, or a
biosensor. The rate can be controlled by manipulating a variety of factors, including
the characteristics of the drug formulation to be delivered (e.g., its viscosity, electric
45 charge, and chemical composition); the dimensions of each microneedle (e.g., its
outer diameter and the area of porous or hollow openings); the number of
microneedles in the device; the application of a driving force (e.g., a concentration
50 gradient, a voltage gradient, a pressure gradient); and the use of a valve.

5 The rate also can be controlled by interposing between the drug in the
reservoir and the opening(s) at the base end of the microneedle polymeric or other
materials selected for their diffusion characteristics. For example, the material
10 composition and layer thickness can be manipulated using methods known in the art
5 to vary the rate of diffusion of the drug of interest through the material, thereby
controlling the rate at which the drug flows from the reservoir through the
microneedle and into the tissue.

15 Transportation of molecules through the microneedles can be controlled or
monitored using, for example, various combinations of valves, pumps, sensors,
10 actuators, and microprocessors. These components can be produced using standard
manufacturing or microfabrication techniques. Actuators that may be useful with the
20 microneedle devices disclosed herein include micropumps, microvalves, and
positioners. In a preferred embodiment, a microprocessor is programmed to control
a pump or valve, thereby controlling the rate of delivery.

25 Flow of molecules through the microneedles can occur based on diffusion,
capillary action, or can be induced using conventional mechanical pumps or
nonmechanical driving forces, such as electroosmosis or electrophoresis, or
convection. For example, in electroosmosis, electrodes are positioned on the
30 biological barrier surface, one or more microneedles, and/or the substrate adjacent
the needles, to create a convective flow which carries oppositely charged ionic
species and/or neutral molecules toward or into the biological barrier. In a preferred
embodiment, the microneedle device is used in combination with another
35 mechanism that enhances the permeability of the biological barrier, for example by
increasing cell uptake or membrane disruption, using electric fields, ultrasound,
25 chemical enhancers, vacuum viruses, pH, heat and/or light.

40 Passage of the microneedles, or drug to be transported via the microneedles,
can be manipulated by shaping the microneedle surface, or by selection of the
material forming the microneedle surface (which could be a coating rather than the
microneedle per se). For example, one or more grooves on the outside surface of the
45 microneedles can be used to direct the passage of drug, particularly in a liquid state.
Alternatively, the physical surface properties of the microneedle can be manipulated
to either promote or inhibit transport of material along the microneedle surface, such
as by controlling hydrophilicity or hydrophobicity.

5 The flow of molecules can be regulated using a wide range of valves or
gates. These valves can be the type that are selectively and repeatedly opened and
closed, or they can be single-use types. For example, in a disposable, single-use
10 drug delivery device, a fracturable barrier or one-way gate may be installed in the
5 device between the reservoir and the opening of the microneedles. When ready to
use, the barrier can be broken or gate opened to permit flow through the
microneedles. Other valves or gates used in the microneedle devices can be
15 activated thermally, electrochemically, mechanically, or magnetically to selectively
initiate, modulate, or stop the flow of molecules through the needles. In a preferred
10 embodiment, flow is controlled by using a rate-limiting membrane as a "valve."

20 The microneedle devices can further include a flowmeter or other means to
monitor flow through the microneedles and to coordinate use of the pumps and
valves.

f. Sensors

25 The sensing/analyzing function can occur in the microneedle or body of the
device (e.g., in the fluid collection chamber), or external to the device following
removal of a sample. The sensing device can be in or attached to one or more
microneedles, integrated into the substrate, or within or in communication with the
30 fluid collection chamber. Biosensors can be located on the microneedle surface.
20 inside a hollow or porous microneedle, or inside a device in communication with the
body tissue via the microneedle (solid, hollow, or porous).

35 In a preferred embodiment, the microneedle device provides a single-use
collection means. In this design, the microneedle array is used to extract a single
measurement and then is detached from a reusable base portion, if any, and
25 disposed.

40 In one embodiment, the microneedle device is adapted to work with
"laboratory-on-a-chip" devices, such as made by Caliper Technologies, Palo Alto,
California (*see, e.g.*, U.S. Patent No. 5,852,495 to Parce and U.S. Patent No.
5,876,675 to Kennedy); Aclara Biosciences, Hayward, California (*see, e.g.*, U.S.
45 Patent No. 5,858,188 to Soane et al. and U.S. Patent No. 5,883,211 to Sassi et al.);
30 and Nanogen, San Diego, California (*see, e.g.*, U.S. Patent Nos. 5,605,662 and
5,632,957 to Heller et al.).

5

(ij. Types of Sensors

10

Useful sensors may include sensors of pressure, temperature, chemicals, pH, and/or electro-magnetic fields. These microneedle biosensors can include four classes of principal transducers: potentiometric, amperometric, optical, and physiochemical. An amperometric sensor monitors currents generated when electrons are exchanged between a biological system and an electrode. Blood glucose sensors frequently are of this type.

15

Sensing information or signals can be transferred optically (e.g., refractive index) or electrically (e.g., measuring changes in electrical impedance, resistance, current, voltage, or combination thereof). For example, it may be useful to measure a change in the resistance of tissue to an electrical current, wherein different resistances are calibrated to signal that withdrawal has been completed.

20

25

In a preferred embodiment, the microneedle device may include an integrated sensor, such as a chemical sensor, biosensor, or other measurement system to form a complete extraction/ measurement system. The unit can be constructed to function as a closed loop drug delivery unit, including drug delivery means, analyte recovery means, sensing means to measure the analyte, and control means to provide a signal to the drug delivery means. In a preferred embodiment, the unit would include subunits to withdraw fluid and calculate the concentration of glucose, for example, to determine the amount of insulin needed and deliver that amount of insulin.

30

20

35

The device can include means for assaying the amount of analyte extracted. For example, an assay method that results in a color change could be used. The change in color could be detected using a light beam that enters into a disposable collection chamber through a window on top. The analyte may also be detected in the chamber through the use of an enzyme electrode or biosensor. The analyte sensing system can include enzymes that react with the analyte of interest and either electrochemical or optical transducers that measure the content of reaction. Examples of such enzymes are glucose oxidase and glucose dehydrogenase.

40

45

An example of an enzyme electrode for glucose is a screen-printed electrode on the surface of which is immobilized glucose oxidase and an electron mediator such as ferrocene or its derivatives. Electrons generated by the oxidation of glucose are transferred from glucose oxidase to the electrode via the mediator. Thus, the

50

55

5 concentration of glucose in the analyte solution is proportional to the current generated. Yet another detection mechanism may be used based on near-infrared spectroscopy. In this method, concentration of extracted glucose in a gel is detected
10 by the absorption of the near-infrared light that passes through the chamber through two windows.

(ii). Microneedle as Sensing Element

15 In one embodiment, the microneedle is adapted to be the sensing element. For example, an assay material, such as glucose oxidase, can be (i) coated onto the external surface of hollow or solid microneedles, (ii) distributed within the pores of
10 porous microneedles, or (iii) line or fill the bore(s) of hollow microneedles. See Figure 27 which illustrates a cross sectional view of a preferred embodiment of a microneedle device 630 including microneedle 632, attached to substrate 634 and
20 having hollow bore 636. In Figure 27a, sensor material 638 is coated on the external surface of microneedle 632. In Figure 27b, sensor material 638 is coated on the internal surface of hollow bore 636. In Figure 27c, sensor material 638 is located
25 within the pores of a porous microneedle 632. Solid microneedles can also hold or contain sensor material as in Figure 27a, or as in Figure 27c if the microneedles are porous. These various microneedle types and sensors can be used in different
30 combinations within a device array.

20 In this embodiment, the assay material contacts the analyte for which it is selective and undergoes a change, such as an oxidation reaction. This change is communicated, either directly or indirectly, to the user. For example, change may
35 be indicated optically (change in color or refractive index) or electrically. Alternatively, the change may induce a shift in pH that can be measured and communicated using conventional techniques. In more complex embodiments, the
25 analyte may be adsorbed to the microneedle or a coating thereon, such that mechanical sensing can be used, for example, by measuring vibration changes caused by the adsorption.

45 The microneedle may function as a conduit for fluids, solutes, electric charge, light, or other materials. In one embodiment, hollow microneedles can be
30 filled with a substance, such as a gel, that has a sensing functionality associated with it. In an application for sensing based on binding to a substrate or reaction mediated by an enzyme, the substrate or enzyme can be immobilized in the needle interior.

5 which would be especially useful in a porous needle to create an integral
needle/sensor.

(iii). Sensor Electronics

10 In a preferred embodiment, the sensors are selectively in communication
5 with an electronics package. The electronics package typically includes a power
source (e.g., a battery), as well as electronic hardware and software for the
transduction, storage, transmission, and display of measured values. The electronics
15 package can be selectively fixed to the microneedle device, for example, so that the
electronics package can be reused with a new, disposable microneedle device. The
10 electronics package can include a mechanism for wireless or wire-based
transmission of measured values to a remote device for analysis and/or display. The
20 electronics also may include mathematical manipulation of the sensed data, for
example, to average measured values or eliminate outlying datapoints so as to
provide more useful measurements.

25 The electronics package also can include software and hardware to initiate or
automate the sensing and analysis processes. It may be desirable to design a
microneedle device capable of taking multiple measurements to withdraw/sense
samples on a preprogrammed schedule (e.g., periodic or random), for example, to
30 monitor the blood plasma levels of an illegal drug. Such a device could be adapted
20 for use with a transmitter designed to lock onto the wrist or ankle of a drug offender
or other probationer. The device would then be able to randomly test the wearer
without his knowledge in order to assess his compliance with orders to abstain from
35 drug or alcohol use.

In an alternative embodiment, the electronics package includes a device for
25 controlling the withdrawal or sensing process. For example, sensing could be
activated based on elapsed time, body temperature, or in response to an external
40 trigger (e.g., motion sensor or push-button). The electronics package, for example,
could provide substantially instantaneous readings of glucose levels by depressing a
button, or in a microneedle device (e.g., adapted to be worn for an extended period
45 of time), the electronics could it could display a summary of intermittent glucose
30 measurements taken automatically throughout the day. Such a microneedle device
would be highly useful to diabetic patients to routinely monitor their blood glucose
levels following insulin dosing, between or following meals, and at other times
50

5 throughout the day.

Wave guides can be incorporated into the microneedle device to direct light to a specific location, or for detection, for example, using means such as a pH dye for color evaluation. Similarly, heat, electricity, light or other energy forms may be precisely transmitted to directly stimulate, damage, or heal a specific tissue or intermediary (e.g., tattoo removal for dark skinned persons), or diagnostic purposes, such as measurement of blood glucose based on IR spectra or by chromatographic means, measuring a color change in the presence of immobilized glucose oxidase in combination with an appropriate substrate.

10 (iv). Single Unit Multiple Sensing

A single microneedle device can be designed to provide multiple, preferably sequential, measurements. In a preferred embodiment, the device includes a plurality of discrete fluid collection chambers, each of which is in communication with a defined subset of microneedles in an array of microneedles. The sensing unit of the device can sense each of the collection chambers independently. The sensing can be triggered manually or device electronics can be preprogrammed to automatically trigger, for example at specific time intervals. The device can include a means for storing, displaying, or transmitting the multiple measured values as needed.

20 (v). Sensor Calibration

Calibration of the sensor can be accomplished using the concentration of a second analyte or the same analyte measured by another means. The primary analyte can be normalized, lowering extraction to extraction and site to site variability, by the concentration of the second analyte or same analyte from a separate measurement. Normalization may be a linear or non-linear relationship.

In a preferred embodiment for glucose sensing, a reusable sensor, which assays glucose concentration in interstitial fluid, can be calibrated daily by correlating interstitial fluid glucose values with values obtained from glucose measurements obtained from blood, similar to the approach used by Cygnus Inc.'s "Gluco-Watch."

30 g. Attachment Features

A collar or flange also can be provided with the device, for example, around the periphery of the substrate or the base. It preferably is attached to the device, but

alternatively can be formed as an integral part of the substrate, for example by forming microneedles only near the center of an "oversized" substrate. The collar can also emanate from other parts of the device. The collar can provide an interface to attach the microneedle array to the rest of the device, and can facilitate handling of the smaller devices.

In a preferred embodiment, the microneedle device includes an adhesive to temporarily secure the device to the surface of the biological barrier. The adhesive can be essentially anywhere on the device to facilitate contact with the biological barrier. For example, the adhesive can be on the surface of the collar (same side as microneedles), on the surface of the substrate between the microneedles (near the base of the microneedles), or a combination thereof.

The device can be integrated into an adhesive patch or an elastic band, which may be worn, for example, around the user's arm or ankle. The arm band can be conveniently worn by a patient for drug delivery, sampling of biological fluids, or both over a prolonged period of time, such as several hours.

Care must be taken so that any adhesive agent does not plug the bores of hollow microneedles. For example, the adhesive agent can be applied in a liquid solution by flooding the top of the substrate below the tips of the microneedles, such as from the side of an array of microneedles, or by using a three-dimensional printing process. The solvent can then be evaporated from the adhesive agent solution, thereby precipitating or gelling the adhesive agent to yield a tacky surface. An alternate method of keeping the tips free of an applied adhesive agent is to choose materials of construction having a hydrophobicity or hydrophilicity to control the wetting of the surface to the microneedle tips.

Where a vacuum is used to induce fluid flow into the device, it may be necessary to provide means for creating a gas-tight seal around the edge of the device so that air is not drawn in through the microneedles at the biological barrier hole/microneedle shaft periphery. The attachment collar or adhesive material can be adapted to provide this function using techniques common to the those skilled in the art. One example is to design the attachment collar to function as a "suction-cup" and wet the interface of the skin and attachment collar with water or another physiologically acceptable sealant.

h. Transdermal Microneedle Device

Figure 9 is a side elevational view of a schematic of an embodiment of the microneedle device inserted into undeformed skin. The device 10 includes an upper portion or substrate 11 from which a plurality of microneedles 12 protrude. The height of the upper portion 11 is between about 1 μm and 1 cm, and the width of the upper portion is between about 1 mm and 10 cm. The upper portion 11 of the device can be solid or hollow, and may include multiple compartments. In a preferred embodiment for drug delivery, the upper portion 11 contains one or more drugs to be delivered. It is also preferred that the upper portion include one or more sensors and/or an apparatus (e.g., pump or electrode) to drive (provide/direct the force) transport of the drug or other molecules.

The height (or length) of the microneedles 12 generally is between about 1 μm and 1 mm. The diameter and length both affect pain as well as functional properties of the needles. In one embodiment for transdermal applications, the "insertion depth" of the microneedles 12 is less than about 100 μm , more preferably about 30 μm , so that insertion of the microneedles 12 into the skin through the stratum corneum 14 does not penetrate through the epidermis 16 into the dermis 18 (as described below), thereby avoiding contacting nerves and reducing the potential for causing pain. In such applications, the actual length of the microneedles may be longer, since the portion of the microneedles distal the tip may not be inserted into the skin: the uninserted length depends on the particular device design and configuration. The actual (overall) height or length of microneedles 12 should be equal to the insertion depth plus the uninserted length. Other embodiments using sufficiently small microneedles may penetrate into the dermis without causing pain.

The diameter of each microneedle 12 generally is between about 10 nm and 1 mm, and preferably leaves a residual hole (following microneedle insertion and withdrawal) of less than about 1 μm , to avoid making a hole which would allow bacteria to enter the penetration wound. The actual microneedle diameter should be larger than 1 μm , since the hole likely will contract following withdrawal of the microneedle. The diameter of microneedle 12 more preferably is between about 1 μm and 100 μm . Larger diameter and longer microneedles are acceptable, so long as the microneedle can penetrate the biological barrier to the desired depth and the hole remaining in the skin or other tissue following withdrawal of the microneedle is

5 sufficiently small, preferably small enough to exclude bacterial entry. The
microneedles 12 can be solid or porous, and can include one or more bores
connected to upper portion 11.

10 i. Microneedle Penetration Enhancing Features

5 In a preferred embodiment, the microneedle devices include features which
improve penetration of the microneedles into deformable, elastic biological barriers,
such as human skin. As used herein, "improved penetration" refers to providing
15 more uniform, better controlled insertion of microneedles, for example, as compared
to manual insertion of a microneedle or array of microneedles into skin without
20 compensation (in the device design or site preparation or both) for deformation of
the skin at the intended site of insertion. This is particularly critical for devices
which include a three dimensional array of the microneedles. These features
typically function to (1) adapt to the deformation, (2) limit the deformation, and/or
25 (3) utilize alternate ways of creating the holes in the biological barrier for the
microneedles to enter. These penetration enhancing techniques generally can be
used with solid, porous, or hollow microneedles. Examples of penetration
enhancing features include the following:

30 (i). Microneedle Extensions

In a preferred embodiment for adapting the device to the elasticity of skin.
35 the microneedles of the device include extensions, also called protrusion enhancers.
One solution to enhance microneedle penetration would be to make the
microneedles much longer. However, very tall, small diameter microneedles would
tend to be structurally fragile. Therefore, a relatively wider, yet tall base is provided
40 between the substrate and the microneedle to increase the length while maintaining
structural integrity of the microneedles. The extensions can be fabricated using the
same microfabrication techniques described herein or other conventional fabrication
techniques, and typically are made integrally with the substrate and microneedles.
45 The extensions can be of any cross-sectional shape, are typically between about 500
µm and 10 mm in height, and generally are at least about 200 µm in diameter for a
single needle/single extension configuration. A single extension can support one or
more microneedles.

The extensions also can be designed to function as a penetration stop or
limiter, to limit the depth of microneedle penetration.

5 Figures 10a-c illustrate several non-limiting embodiments of the extensions.
Device 110 includes substrate 112, extension 114, and microneedle(s) 116. The
10 figures show a single needle/single extension configuration (10a), a multiple
needle/single extension configuration (10b), and a multiple needle/multiple
5 extension configuration (10c). The microneedle devices can include arrays of
microneedles and extensions in essentially any combination and number.

15 Figure 10d illustrates an embodiment of a microneedle device 180 having
extension 182 terminating in microneedle array 184. The device also includes
shoulder 186 and key (cutout) 188, which serve to control stretching of the skin at
10 the site of microneedle insertion to enhance penetration. The skin stretches in key
188 as microneedle device 180 is pushed in, while shoulder 186 simultaneously
20 limits the area of skin being stretched.

(ii). Optimized Microneedle Spacing

25 In another embodiment to adapt to the deformability of skin, the microneedle
device includes arrays of microneedles having spaces between the microneedles or
15 between arrays of microneedles, wherein the spacings permit areas of the skin to fill
the spaces in order to enhance microneedle contact with adjacent areas of the skin.
The spacing is designed to adapt to the skin's radius of curvature to overcome the
30 penetration problem.

20 Figure 19 illustrates a microneedle device 300 having arrays of
microneedles 302 with spaces 304 between the arrays. Spaces 304 have a size
between about one and ten times, preferably between about one and two times, the
35 size of the arrays 302. This spacing effect can be achieved using some
configurations of the microneedle extensions described above.

25 *(iii). Linear and Curved Arrays of Microneedles*

40 In another embodiment for adapting the device to the elasticity of skin, the
microneedles are provided in a curved three dimensional array. For example, the
microneedle device can have a rigid substrate which forms a curved, rather than
planar, surface. The substrate can be, for example, hemispherical or elliptical. The
45 device, by presenting the needles with a curved surface, can provide improved
uniformity of penetration among the microneedles of an array, as illustrated in
Figure 11a. This same effect also can be achieved by varying the height of the
30 microneedles in the array having a planar substrate, as shown in Figure 11b.

5 In a preferred embodiment, two dimensional (i.e. linear) arrays are used. A preferred embodiment of a linear array microneedle device is shown in Figure 11c. Device 220 includes substrate 222, which is formed into a U-shape, and an array of microneedles 224 at the apex of substrate 222. The substrate/microneedle portion is
10 mounted over the end of a slotted holder 226. Molecules for transport through the microneedles 224 flow through one or more slots 228 positioned at the end of the slotted holder 226. The device also includes a fitting portion 230 which is integral with or attached to the slotted holder 226. The fitting portion 230 can be, for
15 example, a female Luer lock for attachment to a conventional syringe. The use of a linear array such as in this device readily deforms the skin at a sharp radius over the tips of the microneedles 224, greatly facilitating their penetration into the skin.

20 In a variation of this embodiment, several linear arrays of microneedles can be combined onto a single fitting portion or holder in order to increase the area of injection. By spacing the arrays on the holder widely enough, the correct skin
25 deformation can be maintained. The spacing is selected to be sufficient to allow the skin or other barrier to reach a relaxed state in the region between the arrays, thus facilitating the correct deformation over each needle array in a manner independent of other arrays.

30 These microneedle devices are fabricated using or adapting the same microfabrication techniques described herein. In one embodiment, microneedle arrays can be fabricated on flexible substrates, which then are mounted onto rigid
35 spherical, cylindrical, or elliptical surfaces.

(iv). Flexible Substrates

40 The substrate also can be flexible so that it deforms with the skin or other barrier upon application of the microneedle array.

45 Figures 18a-b illustrate a preferred embodiment of a microneedle device having a flexible substrate. In this case, device 250 include microneedles 252, which are fabricated on a flexible substrate 254. The substrate is laminated to a preformed membrane bubble 256, such as those which are used as a membrane switch. This
50 laminated structure is attached to holder 258.

The molecules to be delivered, e.g., drug, are contained in a chamber 260 formed between the membrane bubble 256 and the substrate 254. The molecules are sealed inside the chamber either at the laminating step or are filled after lamination.

5 for example, by injection through the membrane. A sponge or similar device (not shown) may be incorporated into the chamber 260 to contain the molecules before insertion and delivery. The sponge device is compressed by the bubble membrane
10 as it turns to its downward position (*see* Figure 18b).

5 In operation, the device 250 is pressed against the skin, wherein the holder 258 positions the microneedles 252 against the skin, as shown in Figure 18a. Then, force is applied to the membrane bubble 256, flipping it through its transition state
15 to the down position. This action applies pressure to the molecules in the chamber 260, expanding the substrate 254 of the microneedle array and pushing the microneedles 252 through the skin. Subsequently, the pressure forces the molecules
20 through the microneedles 252 and into the skin. The change in pressure upon the membrane bubble must occur faster and be larger than can be relieved by the flow of molecules through the microneedles, in order to achieve effective delivery.

In an alternative embodiment, the chamber 260 may include an intermediate
25 septum or equivalent divider (not shown) which can be ruptured or moved to permit the molecules to flow through the microneedles 252. For example, the user applies pressure to the membrane bubble, which pressure first forces the microneedles into the skin, as shown in Figure 18b, and then ruptures the septum to deliver drugs
30 through the needle and into the skin.

20 (v). High Velocity Insertion

In another embodiment, the microneedles are applied to the skin surface at an increased velocity, thereby reducing the time available for the stratum corneum and
35 underlying tissues to deform from contact with the tips of the microneedles. The insertion can be by forcing the microneedles into the skin, forcing the skin into the microneedles, or a combination thereof. This more rapid microneedle/skin contact
25 can occur, for example, by releasing a compressed spring or other elastic device that pushes or pulls the microneedles, or by a rapid burst release of compressed gas against the back of the substrate. Alternatively, the skin could be forced by rapidly
40 pulling a vacuum or pushing the skin from the sides (pinching) at the site of microneedle administration to cause the skin to be pulled up against an array of microneedles. Various combinations of these mechanisms can be used together, and
45 typically are integrated into the microneedle device.

(vi). Limiting Biological Barrier Elasticity

In preferred embodiments for limiting the elasticity/deformation of tissue, the microneedle device includes features suitable for stretching, pulling, or pinching the tissue, particularly skin, to present a more rigid surface in the area to which the microneedles are applied (i.e. penetrate) as illustrated in Figures 12a-c.

It may also be useful to cool the stratum corneum to reduce its elasticity and/or to apply chemicals to the skin surface to "tighten" the skin and reduce its elasticity. For example, the skin surface may be cooled by directing a flow of cold gas through the microneedles onto the skin surface. The flow of cold gas can be generated, for example, from a liquefied gas source such as nitrogen, carbon dioxide, or a refrigerant such as FREON™. The skin also can be cooled by contact with a cooling (e.g., refrigerated) element, such as a plate, or the microneedles themselves can function as the cooling element. The cooling element should provide sufficient local cooling of the stratum corneum so as to stiffen the stratum corneum in the vicinity of each needle sufficiently to enhance penetration. These cooling means can be used independently or in combination with chemical means to tighten the skin. Examples of chemical means include biocompatible organic solvents, such as isopropanol or acetone, which tend to dry out and stiffen the skin surface, or such astringent chemicals that can be topically applied to the skin before microneedle insertion.

(a). suction

Suction can be used to hold the skin in place during the insertion of the microneedle, limiting the deflection and deformation of skin in contact with the tips of the microneedles. Suction also can be used to bring skin in contact with stationary microneedles, and if sufficiently great, can cause the skin to be pierced by the microneedles. The suction may also enhance systemic delivery of drug by increasing blood flow in the area of administration via the microneedles, or may enhance withdrawal of interstitial fluid or blood for analysis/sensing. The suction typically is induced by creating a vacuum on the skin at the site of microneedle application. The vacuum induced is between about 10 and 2000 mm Hg, preferably between about 50 and 300 mm Hg, at the site of application. The suction typically can occur before, simultaneously with, or following insertion of the microneedles.

5 Examples of microneedle devices adapted to create a vacuum are shown in
Figures 13a-c. Figure 13a shows device 120 which includes substrate 122,
microneedle array 124, and reservoir 126, which is partially enclosed by outer
10 chamber 128. Outer chamber 128 includes a port 127 through which air or other
5 fluids within the chamber are withdrawn following, and/or before, contact of the
opening rim 129 to the skin surface. The outer chamber 128 can be made of flexible
or rigid material, and generally is gas impermeable. A source of vacuum, e.g., a
15 vacuum pump, typically is adapted to be in fluid communication with port 127. A
micro-battery-powered vacuum pump can be integrated into the device to provide
10 this function. In another embodiment, device 128 can be evacuated, so that when
triggered, the skin at the site of administration is exposed to the vacuum and is
20 pulled up into the device. This embodiment effects a short pulse of vacuum, without
requiring extra equipment. In another embodiment, a tool can be used to
mechanically create the necessary vacuum upon manual activation.

25 Figure 13b is a variation of the device shown in Figure 13a, wherein device
130 includes two coaxial cylinders, outer cylinder 132 and inner cylinder 134.
Vacuum is induced in the space between the cylinders. Inner cylinder 134
terminates with reservoir 136, substrate 138, and microneedles 140. Outer cylinder
30 132 and its rim 139 function as the outer chamber 128 and opening rim 129 in
20 Figure 13a. Optionally, an overpressure can be applied in the inner cylinder 134 to
facilitate flow, e.g. of drug, from reservoir 136 through the microneedles 140. The
device can be designed to have the inner cylinder 134 and microneedles 140 in a
35 position fixed or movable with respect to the outer cylinder 132, as appropriate. In
other embodiments, the device can have a non-cylindrical shape.

25 A preferred embodiment of a suction device for use with a microneedle array
is shown in Figure 13c. The suction device 200 includes body portion 202 having
40 an inner vacuum ring 204 and an outer vacuum ring 206, separated by a ring-shaped
microneedle array (not shown). The use of coaxial suction rings provides a uniform
deformation force on the skin. The amount of deformation can be controlled by
45 30 varying the absolute and relative sizes of the annular vacuum rings, and by
controlling the amount of vacuum pulled, for example, by a suction pump. The
relative height of the inner and outer rings, and their height relative to the
microneedle array, can be varied to change the skin deformation and consequent

5 pressure onto the microneedle array. In the device shown, molecules, typically as a
fluid, are delivered through a port 208 in the annular ring holding the microneedles,
and to the whole ring-shaped array through a circular fluidics channel 210 adjacent
10 the substrate of the microneedles. The device shown includes a female Luer lock
5 212 for attachment to a conventional syringe, as well as tubing section 214 that can
be used to connect the device to a vacuum pump of some kind, either manually or
power driven.

15 (b). stretching

Stretching can also be used to limit the deflection and deformation of skin in
10 contact with the tips of the microneedles. The stretching can be effected by a
separate device or incorporated as a feature of the microneedle device itself.

20 Figures 14a-b shows one embodiment of a microneedle device that includes
a stretching component. Microneedle device 150 includes flexible stretching cone
152, which includes circular outer rim 156 and surrounds microneedles 154. Figure
25 14a shows device 150 with the stretching cone 152 in its normal, relaxed form and
shape (i.e. no net forces applied to it) resting on the skin surface, with the tips of
microneedles 154 terminating inside stretching cone 152. Figure 14b shows device
150 following application of pressure (e.g., manual pressure) on device 150 toward
30 the skin. As the force is applied, outer rim 156 begins to "flatten" and frictionally
engages the skin surface, stretching the skin away from and perpendicular to the
20 central axis of the stretching cone 152, while the microneedles 154 move into
contact with and then penetrate the skin. The outer rim 156 should be roughened,
35 knurled, have teeth, or be formed of or coated with a sticky or non-slippery material
so as to provide the necessary engagement between the surfaces. Examples of
25 suitable materials include rubbers and synthetic polymers.

40 In another embodiment, the device includes an aperture or other means of
allowing gas trapped between the barrier and the device to escape. Examples of
such apertures include one or more vent holes or slits, for example, through the side
of the stretching cone 152.

45 30 A preferred embodiment is shown in Figure 14c, wherein stretching cone
152 is replaced with a plurality of, e.g., four, hinged stretching elements 153. The
stretching elements stretch the skin laterally as device 150 is pressed down against
the skin. The skin deflection is determined by the length of the stretcher element
50

5 153 relative to the length of the central cylinder 155. Like outer rim 156, the ends of
the stretching elements 153 (distal the hinge end) preferably are roughened or
10 knurled, have teeth, or are formed of or coated with a sticky or non-slippery material
so as to control the friction between the skin and the stretching elements 153.
5 thereby providing an additional means of controlling the stretching force. The
device shown in Figure 14c is connected to a standard female Luer lock 157, for
15 attachment to a standard syringe. In a preferred embodiment, microneedles 154 are
aligned in columns and rows substantially parallel to the stretching element 153, so
as to optimize the stretching force for effective microneedle penetration.

10 In another embodiment, stretching of the skin is accomplished using a
separate ring device, which can be pressed against the skin and then concentrically
20 expanded to stretch the skin within the ring. For example, the ring device can be a
rubber-coated metal band (having diameter x), which is compressed into a coil
(having a diameter less than x). The coiled ring is then pressed against the skin and
25 15 allowed to uncoil (i.e. expand to diameter x again), while frictionally engaging the
skin, thereby stretching it. In a further embodiment, the ring device is configured as
an iris that expands to stretch the skin upon mechanical actuation by engaging an
actuation lever or rotary motion.

30 (c). pinching

20 Pinching can also be used to limit the deflection and deformation of skin in
contact with the tips of the microneedles. In a preferred embodiment, the
microneedle device includes jaws, typically one or more pair, which can be pressed
35 against the skin surface and triggered to close against a segment of skin, as
illustrated in Figures 15a-b. The size of the jaw opening can be selected based on
25 the area of skin to be pinched to facilitate penetration of the microneedle array
selected for use.

40 In Figures 15a-b, microneedle device 160 includes a pair of jaws 164 having
flex or hinge points 168 and tips 166, positioned around microneedles 162. The
Figures show the jaws 164 in the open position (Fig. 15a) and in the closed position
45 30 (Fig. 15b), pinching an area of skin which is drawn against the microneedle 162,
causing the microneedles to penetrate the skin.

50 An alternative embodiment of the clamping device and method is illustrated
in Figure 15c, wherein clamping device 170 is used to pinch the skin and provide a

5 rigid support 172 behind a pinched section of skin, in order to present a surface of
limited deformability for insertion of the microneedles 174. Clamping device 170
10 can be a separate device from the microneedle device 176, or the devices can be
integrated into a single unit.

5 (d). adhesive film assist

The deformation of skin can be reduced by applying a thin, adhesive film
15 over the skin surface at the site of application. The film keeps the skin taut and
limits deformation at the site of microneedle insertion as the microneedles are
pushed through the film and into the skin. This is analogous to the use of a surgical
10 tape that is applied to the skin before making a surgical incision.

20 The adhesive film can include an expandable or shrinkable material that is
triggered to change size or shape prior to microneedle application, so as to stretch
the skin thereby further limiting its deformability. For example, the material can be
water-swellable, and wetted (triggering event) prior to microneedle application. In
25 another example, the material can change form in response to a change in
temperature (triggering event).

The adhesive film must be thin enough for the microneedles to penetrate
30 both the film and the stratum corneum. If hollow microneedles are used, then the
film should fracture upon penetration without substantial clogging of the hollow
20 bore of the microneedles. Alternatively, the film could be formed of a woven or
porous material so that the microneedles substantially penetrate gaps or pores in the
adhesive film rather than the fibers or matrix of the film material. Examples of
35 suitable films include ethylene-tetrafluoroethylene (ETFE) copolymer mesh
(available from Goodfellow PLC) and porous films such as GORETEXTM
25 (available from William H. Gore, Inc.) coupled with an appropriate acrylic adhesive.

40 (vii). Creating Holes for the Microneedles

Another method of improving the penetration of biological barriers with
microneedles involves producing holes or pathways in the barrier through which the
microneedles can traverse, other than the pathway created solely by forcing the
45 microneedle into barrier. A variety of techniques can be adapted for use with the
30 microneedle devices described herein. For example, U.S. Patent No. 5,885,211 to
Eppstein, et al. discloses several methods of selectively removing the stratum
corneum to enhance permeability of human skin. Some of these so-called
50

5 microporation techniques disclosed can be adapted to promote penetration of
microneedles into the viable epidermis. In a preferred embodiment, holes are
created by vaporizing the stratum corneum, for example, by using a laser or by
10 heating of the tips of the microneedles.

5 Laser techniques are described, for example, in U.S. patents No. 5,885,211 to
Eppstein, et al. and No. 4,775,361 to Jacques et al. The laser, or pulsed light source,
preferably is used in conjunction with a dye which substantially absorbs over the
15 emission range of the light. The dye is applied to the skin and the laser or light is
focused on the dye, heating it. Then, the stratum corneum adjacent to the dye is
10 heated by conduction, elevating the temperature of tissue-bound water and other
vaporizable substances in the selected area above the vaporization point of the water
and other vaporizable substances. This vaporization results in degradation of the
stratum corneum at one or more select, i.e. pinpoint, areas, through which the
microneedles can readily penetrate. One of skill in the art can readily select the
25 appropriate dye, laser (e.g., Helium-Neon) or light source, and parameters of use,
based, in part, on the particular microneedle array, drug to be delivered, and/or
analyte to sample. In one embodiment, the light is focused, in part, by passing the
light through the internal bore of a hollow microneedle.

30 Thermal ablation of the stratum corneum can be achieved by radiant heating
(using a light/laser as described above) or by using conductive heating. For
example, U.S. Patent No. 5,885,211 to Eppstein, et al. describes contacting human
skin with a heat source (conductive heating) ablate the stratum corneum. The
35 microneedle devices described herein can be applied to the ablated skin and/or can
be configured to provide the ablation of the stratum corneum, in particularly by
25 heating the microneedles to serve as the heat source which contacts the skin.
Heating of the microneedles can be accomplished, for example, by (1) contacting the
40 needles with an ohmic heating element, (2) providing microneedles formed of or
coated with a conductive material, through which a modulated electrical current is
passed to induce resistive heating of the microneedles, or (3) providing microneedles
45 positioned in a modulatable alternating magnetic field of an excitation coil such that
energizing the excitation coil with alternating current produces eddy currents
sufficient to heat the microneedles by internal ohmic losses. The microneedles
should be able to rapidly heat the skin surface at select spots to above 100 °C.

5 preferably above 123 °C. to induce flash vaporization of the water content of the
stratum corneum, as described in U.S. Patent No. 4,775,361 to Jacques et al. The
heating preferably is done using an on/off cycling technique and/or adjacent cooling
10 to minimize damage to tissues adjacent the target area. In embodiments in which the
microneedles are heated, the substrate preferably includes an insulating material, as
5 shown in Figure 16, which illustrates two hollow microneedles and substrate in
cross-section.

15 Other embodiments include applying a jet or focused blast of high pressure
fluid to hydraulically puncture the stratum corneum and form a micropore into
10 which the microneedle is inserted. The micropore preferably is slightly larger than
the diameter of the microneedle. The microneedle device can be designed to utilize
20 hollow microneedles to direct the jet of high pressure fluid. Various devices and
techniques for high velocity introduction of fluids and particles into skin for delivery
of drugs or genes are described, for example, in U.S. Patents No. 5,919,159 and No.
25 5,599,302 to Lilley, et al. (Medi-Ject, Inc.), U.S. Patent No. 5,899,880 to Bellhouse,
et al. (PowderJect Research Ltd.), and U.S. Patent No. 5,865,796 to McCabe
(PowderJect Vaccines, Inc.). Creation of the holes and penetration can be enhanced
by select cooling/freezing of the surface of the skin, e.g., cryoablation (see U.S.
30 Patent No. 5,147,355 to Friedman, et al.). For example, the microneedle device can
20 be adapted to create a local Joule-Thompson effect (see U.S. Patent No. 5,758,505 to
Dobak III, et al.).

35 In another embodiment, chemical agents, such as certain keratin reducing
agents (see U.S. Pat. No. 5,911,223 to Weaver et al.), can be applied at the site of
administration to degrade the keratin of the skin's stratum corneum, rendering it
25 more porous. Examples of suitable chemicals include sodium thiosulfate and urea.

40 (viii). Lubricated Microneedles

In one embodiment, the microneedles include a lubricating material, such as
TEFLON™ (polytetrafluoroethylene), coated onto the microneedles. In a preferred
embodiment, the lubricating material is incorporated into metal microneedles, for
45 30 example, by plating the lubricating material with the metal during the manufacture
of the microneedles.

(ix). Vibrating the Microneedles

Essentially all of the microneedle devices and methods described herein can be adapted to vibrate the microneedles and/or the skin to further facilitate penetration. The vibration can be effected to move the microneedles perpendicular and/or parallel to the surface of the biological barrier, and/or at an orientation thereinbetween. The vibration motion can be induced using known techniques, the most common of which is coupling the microneedle or array thereof to a piezoelectric transducer that can provide the vibratory motion. Such a transducer can be bonded directly to the array or can be bonded to a reservoir, thereby utilizing the acoustic transmission properties of the reservoir contents (e.g., an aqueous drug solution) to transmit vibration to the microneedles. Alternatively, electromechanical actuation can be used to vibrate the microneedles, such electromechanical actuation means include miniature motors and speaker coils.

3. Methods of Making Microneedle Devices

The microneedle devices are made by microfabrication processes, by creating small mechanical structures in silicon, metal, polymer, and other materials. These microfabrication processes are based on well-established methods used to make integrated circuits, electronic packages and other microelectronic devices, augmented by additional methods used in the field of micromachining. The microneedle devices can have dimensions as small as a few nanometers and can be mass-produced at low per-unit costs.

a. Microfabrication Processes

Microfabrication processes that may be used in making the microneedles disclosed herein include lithography; etching techniques, such as wet chemical, dry, and photoresist removal; thermal oxidation of silicon; electroplating and electroless plating; diffusion processes, such as boron, phosphorus, arsenic, and antimony diffusion; ion implantation; film deposition, such as evaporation (filament, electron beam, flash, and shadowing and step coverage), sputtering, chemical vapor deposition (CVD), epitaxy (vapor phase, liquid phase, and molecular beam), electroplating, screen printing, lamination, stereolithography, laser machining, and laser ablation (including projection ablation). See generally Jaeger, Introduction to Microelectronic Fabrication (Addison-Wesley Publishing Co., Reading MA 1988); Runyan, *et al.*, Semiconductor Integrated Circuit Processing Technology (Addison-

5 Wesley Publishing Co., Reading MA 1990); *Proceedings of the IEEE Micro Electro Mechanical Systems Conference 1987-1998*; Rai-Choudhury, ed., Handbook of
10 Microlithography, Micromachining & Microfabrication (SPIE Optical Engineering Press, Bellingham, WA 1997).

5 The following methods are preferred for making microneedles.

(i). Electrochemical Etching of Silicon

15 In this method, electrochemical etching of solid silicon to porous silicon is used to create extremely fine (on the order of 0.01 μm) silicon networks which can be used as piercing structures. This method uses electrolytic anodization of silicon
10 in aqueous hydrofluoric acid, potentially in combination with light, to etch channels into the silicon. By varying the doping concentration of the silicon wafer to be etched, the electrolytic potential during etching, the incident light intensity, and the electrolyte concentration, control over the ultimate pore structure can be achieved.
20 The material not etched (i.e. the silicon remaining) forms the microneedles. This method has been used to produce irregular needle-type structures measuring tens of
25 nanometers in width.

(ii). Plasma Etching

30 This process uses deep plasma etching of silicon to create microneedles with diameters on the order of 0.1 μm or larger. Needles are patterned directly using
20 photolithography, rather than indirectly by controlling the voltage (as in electrochemical etching), thus providing greater control over the final microneedle geometry.

35 In this process, an appropriate masking material (e.g., metal) is deposited onto a silicon wafer substrate and patterned into dots having the diameter of the
25 desired microneedles. The wafer is then subjected to a carefully controlled plasma based on fluorine/oxygen chemistries to etch very deep, high aspect ratio trenches into the silicon. See, e.g., Jansen, *et al.*, "The Black Silicon Method IV: The Fabrication of Three-Dimensional Structures in Silicon with High Aspect Ratios for Scanning Probe Microscopy and Other Applications," *IEEE Proceedings of Micro*
40 *Electro Mechanical Systems Conference*, pp. 88-93 (1995). Those regions protected by the metal mask remain and form the needles. This method is further described in Example 1 below.

(iii). Electroplating

In this process, a metal layer is first evaporated onto a planar substrate. A layer of photoresist is then deposited onto the metal to form a patterned mold which leaves an exposed-metal region in the shape of needles. By electroplating onto the exposed regions of the metal seed layer, the mold bounded by photoresist can be filled with electroplated material. Finally, the substrate and photoresist mold are removed, leaving the finished microneedle array. The microneedles produced by this process generally have diameters on the order of 1 μm or larger. See, e.g., Frazier, *et al.*, "Two dimensional metallic microelectrode arrays for extracellular stimulation and recording of neurons", *IEEE Proceedings of the Micro Electro Mechanical Systems Conference*, pp. 195-200 (1993).

(iv). Other Processes

Another method for forming microneedles made of silicon or other materials is to use microfabrication techniques such as photolithography, plasma etching, or laser ablation to make a mold form (A), transferring that mold form to other materials using standard mold transfer techniques, such as embossing or injection molding (B), and reproducing the shape of the original mold form (A) using the newly-created mold (B) to yield the final microneedles (C). Alternatively, the creation of the mold form (A) could be skipped and the mold (B) could be microfabricated directly, which could then be used to create the final microneedles (C).

Another method of forming solid silicon microneedles is by using epitaxial growth on silicon substrates, as is utilized by Containerless Research, Inc. (Evanston, Illinois, USA) for its products.

b. Hollow or Porous Microneedles

In a preferred embodiment, microneedles are made with pores or other pathways through which material may be transported. The following descriptions outline representative methods for fabricating either porous or hollow microneedles.

(i). Porous Microneedles

Rather than having a single, well-defined hole down the length of the needle, porous needles are filled with a network of channels or pores which allow conduction of fluid or energy through the needle shaft. It has been shown that by appropriate electrochemical oxidation of silicon, pore arrays with high aspect ratios

5 and a range of different pore size regimes can be formed; these pore regimes are
defined as (1) microporous regime with average pore dimensions less than 2 nm, (2)
mesoporous regime with average pore sizes of between 2 nm and 50 nm, and (3)
10 macroporous regime with pores greater than 50 nm. The mesoporous and
5 macroporous regimes are expected to be most useful for drug delivery. Two
approaches to porous needles are generally available, either (a) the silicon wafer is
first made porous and then etched as described above to form needles or (b) solid
15 microneedles are etched and then rendered porous, for example, by means of
electrochemical oxidation, such as by anodization of a silicon substrate in a
10 hydrofluoric acid electrolyte. The size distribution of the etched porous structure is
highly dependent on several variables, including doping kind and illumination
conditions, as detailed in Lehmann, "Porous Silicon--A New Material for MEMS",
20 *IEEE Proceedings of the Micro Electro Mechanical Systems Conference*, pp. 1-6
(1996). Porous polymer or metallic microneedles can be formed, for example, by
25 micromolding a polymer containing a volatilizable or leachable material, such as a
volatile salt, dispersed in the polymer or metal, and then volatilizing or leaching the
dispersed material, leaving a porous polymer matrix in the shape of the microneedle.

30 (ii). Hollow Microneedles

Three-dimensional arrays of hollow microneedles can be fabricated, for
20 example, using combinations of dry etching processes (Laermer, et al., "Bosch Deep
Silicon Etching: Improving Uniformity and Etch Rate for Advanced MEMS
Applications," *Micro Electro Mechanical Systems*, Orlando, FL, USA, (Jan. 17-21,
35 1999); Despont et al., "High-Aspect-Ratio, Ultrathick, Negative-Tone Near-UV
Photoresist for MEMS", *Proc. of IEEE 10th Annual International Workshop on*
25 *MEMS*, Nagoya, Japan, pp. 518-22 (Jan. 26-30, 1997)); micromold creation in
lithographically-defined and/or laser ablated polymers and selective sidewall
40 electroplating; or direct micromolding techniques using epoxy mold transfers.

One or more distinct and continuous pathways are created through the
interior of microneedles. In a preferred embodiment, the microneedle has a single
45 30 annular pathway along the center axis of the microneedle. This pathway can be
achieved by initially chemically or physically etching the holes in the material and
then etching away microneedles around the hole. Alternatively, the microneedles
and their holes can be made simultaneously or holes can be etched into existing
50

microneedles. As another option, a microneedle form or mold can be made, then coated, and then etched away, leaving only the outer coating to form a hollow microneedle. Coatings can be formed either by deposition of a film or by oxidation of the silicon microneedles to a specific thickness, followed by removal of the interior silicon. Also, holes from the backside of the wafer to the underside of the hollow needles can be created using a front-to-backside infrared alignment followed by etching from the backside of the wafer.

(a). silicon microneedles

One method for hollow needle fabrication is to replace the solid mask used in the formation of solid needles by a mask that includes a solid shape with one or more interior regions of the solid shape removed. One example is a "donut-shaped" mask. Using this type of mask, interior regions of the needle are etched simultaneously with their side walls. Due to lateral etching of the inner side walls of the needle, this may not produce sufficiently sharp walls. In that case, two plasma etches may be used, one to form the outer walls of the microneedle (i.e., the 'standard' etch), and one to form the inner hollow core (which is an extremely anisotropic etch, such as in inductively-coupled-plasma "ICP" etch). For example, the ICP etch can be used to form the interior region of the needle followed by a second photolithography step and a standard etch to form the outer walls of the microneedle. Figure 1a represents a silicon wafer 82 with a patterned photoresist layer 84 on top of the wafer 82. The wafer 82 is anisotropically etched (Figure 1b) to form a cavity 86 through its entire thickness (Figure 1c). The wafer 82 is then coated with a chromium layer 88 followed by a second photoresist layer 90 patterned so as to cover the cavity 86 and form a circular mask for subsequent etching (Figure 1d). The wafer 82 is then etched by a standard etch to form the outer tapered walls 92 of the microneedle (Figure 1e).

Alternatively, this structure can be achieved by substituting the chromium mask used for the solid microneedles described in Example 1 by a silicon nitride layer 94 on the silicon substrate 95 covered with chromium 96, deposited as shown in Figure 2a and patterned as shown in Figure 2b. Solid microneedles are then etched as described in Example 1 as shown Figure 2c, the chromium 96 is stripped (Figure 2d), and the silicon 95 is oxidized to form a thin layer of silicon dioxide 97 on all exposed silicon surfaces (Figure 2e). The silicon nitride layer 94 prevents

5 oxidation at the needle tip. The silicon nitride 94 is then stripped (Figure 2f),
leaving exposed silicon at the tip of the needle and oxide-covered silicon 97
everywhere else. The needle is then exposed to an ICP plasma which selectively
10 etches the inner sidewalls of the silicon 95 in a highly anisotropic manner to form
5 the interior hole of the needle (Figure 2g).

Another method uses the solid silicon needles described previously as 'forms'
around which the actual needle structures are deposited. After deposition, the forms
15 are etched away, yielding the hollow structures. Silica needles or metal needles can
be formed using different methods. Silica needles can be formed by creating needle
10 structures similar to the ICP needles described above prior to the oxidation described
above. The wafers are then oxidized to a controlled thickness, forming a layer on
20 the shaft of the needle form which will eventually become the hollow microneedle.
The silicon nitride is then stripped and the silicon core selectively etched away (e.g.,
in a wet alkaline solution) to form a hollow silica microneedle.

25 In a preferred embodiment, an array of hollow silicon microtubes is made
using deep reactive ion etching combined with a modified black silicon process in a
conventional reactive ion etcher, as described in Example 3 below. First, arrays of
circular holes are patterned through photoresist into SiO_2 , such as on a silicon
30 wafer. Then the silicon can be etched using deep reactive ion etching (DRIE) in an
inductively coupled plasma (ICP) reactor to etch deep vertical holes. The
photoresist was then removed. Next, a second photolithography step patterns the
remaining SiO_2 layer into circles concentric to the holes, leaving ring shaped oxide
35 masks surrounding the holes. The photoresist is then removed and the silicon wafer
again deep silicon etched, such that the holes are etched completely through the
25 wafer (inside the SiO_2 ring) and simultaneously the silicon is etched around the SiO_2
ring leaving a cylinder.

40 This latter process can be varied to produce hollow, tapered microneedles.
After an array of holes is fabricated as described above, the photoresist and SiO_2
layers are replaced with conformal DC sputtered chromium rings. The second ICP
45 etch is replaced with a SF_6/O_2 plasma etch in a reactive ion etcher (RIE), which
30 results in positively sloping outer sidewalls. Henry, et al., "Micromachined Needles
for the Transdermal Delivery of Drugs," *Micro Electro Mechanical Systems*,
Heidelberg, Germany, pp. 494-98 (Jan. 26-29, 1998).

5

(b). metal microneedles

10

15

20

Metal needles can be formed by physical vapor deposition of appropriate metal layers on solid needle forms, which can be made of silicon using the techniques described above, or which can be formed using other standard mold techniques such as embossing or injection molding. The metals are selectively removed from the tips of the needles using electropolishing techniques, in which an applied anodic potential in an electrolytic solution will cause dissolution of metals more rapidly at sharp points, due to concentration of electric field lines at the sharp points. Once the underlying silicon needle forms have been exposed at the tips, the silicon is selectively etched away to form hollow metallic needle structures. This process could also be used to make hollow needles made from other materials by depositing a material other than metal on the needle forms and following the procedure described above.

25

30

35

40

45

50

A preferred method of fabricating hollow metal microneedles utilizes micromold plating techniques, which are described as follows and in Examples 4 and 5. In a method for making metal microtubes, which does not require dry silicon etching, a photo-defined mold first is first produced, for example, by spin casting a thick layer, typically 150 μm , of an epoxy (e.g., SU-8) onto a substrate that has been coated with a thin sacrificial layer, typically about 10 to 50 nm. Arrays of cylindrical holes are then photolithographically defined through the epoxy layer, which typically is about 150 μm thick. (Despont, et al., "High-Aspect-Ratio, Ultrathick, Negative-Tone Near-UV Photoresist for MEMS," *Proc. of IEEE 10th Annual International Workshop on MEMS*, Nagoya, Japan, pp. 518-22 (Jan. 26-30, 1997)). The diameter of these cylindrical holes defines the outer diameter of the tubes. The upper surface of the substrate, the sacrificial layer, is then partially removed at the bottom of the cylindrical holes in the photoresist. The exact method chosen depends on the choice of substrate. For example, the process has been successfully performed on silicon and glass substrates (in which the upper surface is etched using isotropic wet or dry etching techniques) and copper-clad printed wiring board substrates. In the latter case, the copper laminate is selectively removed using wet etching. Then a seed layer, such as Ti/Cu/Ti (e.g., 30 nm/200 nm/30 nm), is conformally DC sputter-deposited onto the upper surface of the epoxy mold and onto the sidewalls of the cylindrical holes. The seed layer should be electrically

55

5 isolated from the substrate. Subsequently, one or more electroplatable metals or
alloys are electroplated onto the seed layer. Representative suitable metals and
10 alloys include Ni, NiFe, Au, Cu, Cr, Pt, Pd, and Ti. The surrounding epoxy is then
removed, leaving microtubes which each have an interior annular hole that extends
5 through the base metal supporting the tubes. The rate and duration of electroplating
is controlled in order to define the wall thickness and inner diameter of the
microtubes. In one embodiment, this method was used to produce microtubes
15 having a height of between about 150 and 250 μm , an outer diameter of between
about 40 and 120 μm , and an inner diameter of between about 30 and 110 μm (i.e.,
10 having a wall thickness of 10 μm). In a typical array, the microtubes have a tube
center-to-center spacing of about 150 μm , but can vary depending on the desired
20 needle density.

A variation of this method is preferred for forming tapered microneedles. As
described above, photolithography yields holes in the epoxy which have vertical
25 sidewalls, such that the resulting shafts of the microneedles are straight, not tapered.
This vertical sidewall limitation can be overcome by molding a preexisting 3D
structure, i.e., a mold-insert. The subsequent removal of the mold-insert leaves a
30 mold which can be surface plated similarly to the holes produced by
photolithography described above.

20 Alternatively, non-vertical sidewalls can be produced directly in the
polymeric mold into which electroplating will take place. For example,
35 conventional photoresists known in the art can be exposed and developed in such as
way as to have the surface immediately adjacent to the mask be wider than the other
surface. Specialized greyscale photoresists in combination with greyscale masks can
25 accomplish the same effect. Laser-ablated molds can also be made with tapered
sidewalls, e.g., by optical adjustment of the beam (in the case of serial hole
40 fabrication) or of the reticle or mold during ablation (in the case of projection
ablation).

To form hollow tapered microneedles, the mold-insert is an array of solid
45 30 silicon microneedles, formed as described in Henry, et al., "Micromachined Needles
for the Transdermal Delivery of Drugs," *Micro Electro Mechanical Systems*,
Heidelberg, Germany, Jan. 26-29, pp. 494-98 (1998). First, a layer of a material,
50 such as an epoxy (e.g., SU-8 or a polydimethylsiloxane ("PDMS")), is spin cast onto

the array of silicon needles to completely blanket the entire array. The epoxy settles during pre-bake to create a planar surface above the silicon needle tips; the material is then fully pre-baked, photolithographically cross-linked, and post-baked.

The upper surface of the epoxy is then etched away, for example with an O_2/CHF_3 plasma, until the needle tips are exposed, preferably leaving between about 1 and 5 μm of tip protruding from the epoxy. The silicon is then selectively removed, for example by using a SF_6 plasma or a HNO_3/HF solution. The remaining epoxy micromold is the negative of the microneedles and has a small diameter hole where the tip of the microneedle formerly protruded.

After the removal of the silicon, a seed layer, such as Ti-Cu-Ti, is conformally sputter-deposited onto the epoxy micromold. Following the same process sequence described for hollow metal microtubes, one or more electroplatable metals or alloys, such as Ni, NiFe, Au, or Cu, are electroplated onto the seed layer. Finally, the epoxy is removed, for example by using an O_2/CHF_3 plasma, leaving an array of hollow metal microneedles. An advantage of using PDMS in this application is that the micromold can be physically removed from the silicon mold insert by mechanical means, such as peeling, without damaging the silicon mold insert, thus allowing the silicon mold insert to be reused. Furthermore, the electroplated microneedles can be removed from the PDMS mold by mechanical means, for example by peeling, thereby allowing the PDMS to also be reused. In a preferred embodiment, this method is used to produce microneedles having a height of between about 150 and 250 μm , an outer diameter of between about 40 and 120 μm , and an inner diameter of between about 50 and 100 μm . In a typical array, the microtubes have a tube center-to-center spacing of about 150 μm , but can vary depending on the desired needle density. The microneedles are 150 μm in height with a base diameter of 80 μm , a tip diameter of 10 μm , and a needle-to-needle spacing of 150 μm .

(c). silicon dioxide microneedles

Hollow microneedles formed of silicon dioxide can be made by oxidizing the surface of the silicon microneedle forms (as described above), rather than depositing a metal and then etching away the solid needle forms to leave the hollow silicon dioxide structures. This method is illustrated in Figures 3a-d. Figure 3a shows an

5 array 24 of needle forms 26 with masks 28 on their tips. In Figure 3b, the needle
forms 26 have been coated with a layer 30 of metal, silicon dioxide or other
material. Figure 3c shows the coated needle forms 26 with the masks 28 removed.
10 Finally, in Figure 3d, the needle forms 26 have been etched away, leaving hollow
5 needles 30 made of metal, silicon dioxide, or other materials.

In one embodiment, hollow, porous, or solid microneedles are provided with
longitudinal grooves or other modifications to the exterior surface of the
15 microneedles. Grooves, for example, should be useful in directing the flow of
molecules along the outside of microneedles.

10 (d). polymer microneedles

In a preferred method, polymeric microneedles are made using
microfabricated molds. For example, the epoxy molds can be made as described
above and injection molding techniques can be applied to form the microneedles in
the molds (Weber, et al., "Micromolding - a powerful tool for the large scale
25 production of precise microstructures", *Proc. SPIE - International Soc. Optical
Engineer.* 2879:156-67 (1996); Schiff, et al., "Fabrication of replicated high
precision insert elements for micro-optical bench arrangements" *Proc. SPIE -
International Soc. Optical Engineer.* 3513:122-34 (1998)). These micromolding
30 techniques are preferred over other techniques described herein, since they can
provide relatively less expensive replication, i.e. lower cost of mass production. In a
20 preferred embodiment, the polymer is biodegradable.

Microneedles, particularly hollow ones and ones formed of relatively brittle
35 materials, may break at the juncture of the microneedle and substrate due to
mechanical stresses at the sharp angle formed there. It has been found that the
25 integrity of such microneedles can be improved by reinforcing the base of the
microneedles with an additional layer of material (e.g., silicon) applied onto the face
40 of the substrate face adjacent the base end of the microneedles as shown in Figure
17.

4. **Microneedle Device Applications**

45 30 The device may be used for single or multiple uses for rapid transport across
a biological barrier or may be left in place for longer times (e.g., hours or days) for
long-term transport of molecules. Depending on the dimensions of the device, the
application site, and the route in which the device is introduced into (or onto) the
50

5 biological barrier, the device may be used to introduce or remove molecules at specific locations.

10 As discussed above, Figure 9 shows a side elevational view of a schematic of a preferred embodiment of the microneedle device 10 in a transdermal application.

5 The device 10 is applied to the skin such that the microneedles 12 penetrate through the stratum corneum and enter the viable epidermis so that the tip of the microneedle at least penetrates into the viable epidermis. In a preferred embodiment, drug
15 molecules in a reservoir within the upper portion 11 flow through or around the microneedles and into the viable epidermis, where the drug molecules then diffuse
10 into the dermis for local treatment or for transport through the body.

20 To control the transport of material out of or into the device through the microneedles, a variety of forces or mechanisms can be employed. These include pressure gradients, concentration gradients, electricity, ultrasound, receptor binding, heat, chemicals, and chemical reactions. Mechanical or other gates in conjunction
25 15 with the forces and mechanisms described above can be used to selectively control transport of the material.

In particular embodiments, the device should be "user-friendly." For example, in some transdermal applications, affixing the device to the skin should be
30 relatively simple, and not require special skills. This embodiment of a microneedle
20 may include an array of microneedles attached to a housing containing drug in an internal reservoir, wherein the housing has a bioadhesive coating around the microneedles. The patient can remove a peel-away backing to expose an adhesive
35 coating, and then press the device onto a clean part of the skin, leaving it to administer drug over the course of, for example, several days.

25 a. Drug Delivery

40 Essentially any drug or other bioactive agents can be delivered using these devices. Many drugs can be delivered at a variety of therapeutic rates. The rate can be controlled by varying a number of design factors, including the outer diameter of the microneedle, the number and size of pores or channels in each microneedle, the
45 30 number of microneedles in an array, the magnitude and frequency of application of the force driving the drug through the microneedle and/or the holes created by the microneedles. For example, devices designed to deliver drug at different rates might have more microneedles for more rapid delivery and fewer microneedles for less
50

5 rapid delivery. As another example, a device designed to deliver drug at a variable
rate could vary the driving force (e.g., pressure gradient controlled by a pump) for
transport according to a schedule which was pre-programmed or controlled by, for
10 example, the user or his doctor. The devices can be affixed to the skin or other
5 tissue to deliver drugs continuously or intermittently, for durations ranging from a
few seconds to several hours or days.

One of skill in the art can measure the rate of drug delivery for particular
15 microneedle devices using *in vitro* and *in vivo* methods known in the art. For
example, to measure the rate of transdermal drug delivery, human cadaver skin
10 mounted on standard diffusion chambers can be used to predict actual rates. *See*
Hadgraft & Guy, eds., Transdermal Drug Delivery: Developmental Issues and
20 Research Initiatives (Marcel Dekker, New York 1989); Bronaugh & Maibach,
Percutaneous Absorption, Mechanisms--Methodology--Drug Delivery (Marcel
Dekker, New York 1989). After filling the compartment on the dermis side of the
25 diffusion chamber with saline, a microneedle array is inserted into the stratum
corneum; a drug solution is placed in the reservoir of the microneedle device; and
samples of the saline solution are taken over time and assayed to determine the rates
of drug transport.

30 In an alternate embodiment, biodegradable or non-biodegradable
20 microneedles can be used as the entire drug delivery device, where biodegradable
microneedles are a preferred embodiment. For example, the microneedles may be
formed of a biodegradable polymer containing a dispersion of an active agent for
35 local or systemic delivery. The agent could be released over time, according to a
profile determined by the composition and geometry of the microneedles, the
25 concentration of the drug and other factors. In this way, the drug reservoir is within
the matrix of one or more of the microneedles.

40 In another alternate embodiment, these microneedles may be purposefully
sheared off from the substrate after penetrating the biological barrier. In this way, a
portion of the microneedles would remain within or on the other side of the
45 biological barrier and a portion of the microneedles and their substrate would be
removed from the biological barrier. In the case of skin, this can involve inserting
30 an array into the skin, manually or otherwise breaking off the microneedles tips and
then removing the base of the microneedles. The portion of the microneedles which

5 remains in the skin or other biological barrier can then release drug over time
according to a profile determined by the composition and geometry of the
microneedles, the concentration of the drug and other factors. In a preferred
10 embodiment, the microneedles are made of a biodegradable polymer. The release of
5 drug from the biodegradable microneedle tips can be controlled by the rate of
polymer degradation. The tips can release drugs for local or systemic effect, or
other agents, such as perfume, insect repellent and sun block.

15 Microneedle shape and content can be designed to control the breakage of
microneedles. For example, a notch can be introduced into microneedles either at
20 the time of fabrication or as a subsequent step. In this way, microneedles would
preferentially break at the site of the notch. Moreover, the size and shape of the
portion of microneedles which break off can be controlled not only for specific drug
release patterns, but also for specific interactions with cells in the body. For
example, objects of a few microns in size are known to be taken up by macrophages.
25 The portions of microneedles that break off can be controlled to be bigger or smaller
than that to prevent uptake by macrophages or can be that size to promote uptake by
macrophages, which can be desirable for delivery of vaccines.

(i). Drugs to be Delivered

30 Essentially any drug can be delivered using the microneedle devices. As
20 used herein, the term "drug" refers to an agent which possesses therapeutic,
prophylactic, or diagnostic properties *in vivo*, for example when administered to an
animal, including mammals, such as humans. The drug can be for local treatment or
35 for regional or systemic therapy.

Representative examples of suitable therapeutic and/or prophylactic active
25 agents include proteins, such as hormones, antigens, and growth factors; nucleic
acids, such as antisense molecules; and smaller molecules, such as antibiotics,
40 steroids, decongestants, neuroactive agents, anesthetics, and sedatives. Examples of
suitable diagnostic agents include radioactive isotopes and radioopaque agents,
metals, gases, labels including chromatographic, fluorescent or enzymatic labels.

45 30 The drug can be or include a peptide, protein, carbohydrate (including
monosaccharides, oligosaccharides, and polysaccharides), nucleoprotein,
mucoprotein, lipoprotein, glycoprotein, nucleic acid molecules (including any form
of DNA such as cDNA, RNA, or a fragment thereof, oligonucleotides, and genes).

5 nucleotide, nucleoside, lipid, biologically active organic or inorganic molecules, or combination thereof.

10 Drugs can be selected, for example, from enzymes, polysaccharides, polynucleotide molecules, and synthetic organic and inorganic compounds. Representative agents
5 include anti-infectives, hormones, such as insulin, growth regulators, drugs regulating cardiac action or blood flow, and drugs for pain control. The following are representative examples, and disorders they are used to treat: Calcitonin,
15 osteoporosis; Enoxaprin, anticoagulant; Etanercept, rheumatoid arthritis; Erythropoietin, anemia; Fentanyl, postoperative and chronic pain; Filgrastin, low
10 white blood cells from chemotherapy; Heparin, anticoagulant; Insulin, human, diabetes; Interferon β 1a, multiple sclerosis; Lidocaine, local anesthesia;
20 Somatropin, growth hormone; and Sumatriptan, migraine headaches.

The amount of drug can be selected by one of skill in the art based, for example on the particular drug, its desired effect at the planned release levels, and
25 the time span over which the drug should be released.

(ii). Examples of Drug Delivery Devices

Preferred embodiments of the microneedle device are shown in Figures 20a-
c. The device 510 includes substrate 512 from which a three-dimensional array of
30 microneedles 514 protrude. As shown, the annular bore of the microneedles 514
20 extends through the substrate 512. The device 510 also includes a reservoir 516
secured to substrate 512 via a sealing mechanism 518. Figure 20a shows how the
reservoir can be accessed directly by application to the skin, for example, for simple
35 transdermal delivery of an agent. The device in Figure 20b includes a deformable
bubble reservoir 516. Manual pressure can be used to expel its contents at the site of
25 application. Figure 20c shows a separate reservoir 516 from means 519 for
expelling the contents of the reservoir 516 at the site of administration. The
40 expelling means 519 can be simply a flexible bag. The expelling means 519 may
also contain a vacuum so that it expands when vented, to create pressure on the
reservoir, or it may be elastic so that it deforms when released from one position
45 (not shown). Alternatively, reservoir 516 could be formed of an elastic material
30 which deforms when released.

The sealing mechanism 518 can be, for example, an adhesive material or
gasket. The sealing mechanism 518 can further function as or include a fracturable
50

5 barrier or rate controlling membrane overlaying the surface of the substrate. In this embodiment, nothing can be released until a seal or peel-off strip covering is removed.

10 Another preferred embodiment of the microneedle device is shown in Figure 21. The device 520 includes substrate 512 from which a three-dimensional array of microneedles 514 protrude. The device 520 also includes plunger 522 that is slidably secured to the upper surface of substrate 512 by plunger guide frame 524 using a restraint such as a Leur-lock interface 523. The substrate 512 can be attached or detached to a syringe 526 via a connector such as a Luer-lock type attachment 523. The plunger 522, guide frame 524, and connector 523 connect to, form or contain reservoir 516. A Luer-lock type attachment could alternatively be used to secure the device to means for controlling flow or transport through the device such as a pump.

25 A further preferred embodiment of the microneedle device is shown in Figure 22. Like the device in Figure 21, the device 530 includes substrate 512, microneedles 514, plunger 522, plunger guide frame 524, and reservoir 516. Device 530 further includes plunger housing 532, which is attached to, or integrally formed with, plunger guide frame 524. A compressed spring or other tension-based mechanism 534 is positioned between plunger housing 532 and plunger 522. The device 530 further includes spring hold/release mechanism 536, which keeps the plunger up (spring compressed) until triggered to compress reservoir 516.

35 *(iii). Initiating Delivery*

In a preferred embodiment, delivery of the drug from the reservoir is initiated by applying a force, such as by pressing the top of the reservoir, to cause the reservoir contents (i.e. a drug containing composition) to flow out through the microneedles—an active or dynamic process. For example, the user can apply finger-pressure directly to a deformable reservoir “bubble,” (Figure 20) or to a plunger mechanism (Figure 21) or a Luer-lock type syringe that in turn causes the drug composition to be forced from the reservoir. The plunger also can be adapted to activate by application of a constant, reproducible force, for example, a spring (e.g., under compression) (Figure 22) or elastic band (e.g., in tension).

A variation of this embodiment utilizes a balloon-like reservoir in tension to provide the force. Then, when an opening is formed in the balloon reservoir, the

5 contents are forced out of the reservoir as the balloon contracts to its relaxed state. The contraction is selectively triggered to provide the driving force for delivery.

10 In a preferred embodiment, the force ruptures a fracturable barrier between the reservoir contents and the inlet of the microneedle. Representative barriers
5 include thin foil, polymer, or laminant films. In another preferred embodiment, the microneedles tips are blocked until immediately before use. The blocking material can be, for example, a peelable adhesive or gel film, which will not clog the
15 openings in the microneedle tip when the film is removed from the device.

20 Delivery also can be initiated by opening a mechanical gate or valve interposed between the reservoir outlet and the microneedle inlet. For example, a thin film or plate can be slid or peeled away from the back of the substrate.

25 In an alternate embodiment, delivery is initiated by changing the physical or chemical properties of the drug composition and/or of a barrier material. For example, the barrier can be a porous membrane having a porosity that can be
30 selectably altered to permit flow, or the drug composition can be selected to change from a solid or semi-solid state to a fluid state, for example as the temperature is increased from ambient to that of body temperature. Such a drug composition can be prepared, for example, by combining the drug with a biodegradable polymeric material.

35 A preferred embodiment of the microneedle device is shown in Figure 23a. Figure 23a shows a device 540 in which microneedles 514 attached to a substrate 512 which is attached to multiple compartments 516a, 516b, 516c, and 516d. Each compartment can contain or function as a reservoir. Material can be expelled from each compartment through all or a subset of microneedles 514.

40 Figure 23b depicts a device 550 in which microneedles 514 are attached to a substrate 512 which is attached to reservoir 558 containing, for example, lyophilized drug 554. The reservoir 558 is attached to a fracturable barrier 552 which is attached to another reservoir 556 containing, for example, saline. If the barrier 552 is fractured, the two reservoirs 554 and 556 are in fluid communication with each
45 other and their contents can mix.

50 Delivery also can be initiated by activating an osmotic pump, as described, for example, in U.S. Patent No. 4,320,758 to Eckenhoff, which has been adapted to the substrate of the microneedle device. For example, the reservoir/osmotic pump

5 includes an inner flexible bag that holds the drug charge, an intermediate layer of an
osmotically effective solute composition, such as an inorganic salt, that encapsulates
the bag, and an outer shape-retaining membrane that is at least in part permeable to
10 water and that encapsulates both the layer of osmotically effective solute
5 composition and the bag. In operation, the bag filled with the fluid drug
compositions is exposed to an aqueous environment, so that water is imbibed from
the environment by the osmotically effective solute through the membrane into the
15 space between the inner flexible bag and the membrane. Since the bag is flexible
and the membrane is rigid, the imbibed water squeezes the bag inwardly, thereby
10 displacing drug out the microneedles.

20 Figure 24 shows a device 560 in which microneedles 514 are attached to a
substrate 512 which is attached to a drug reservoir 562. This reservoir is surrounded
at least partially by a flexible, impermeable membrane 564. The drug reservoir is
connected to another reservoir 566 which contains, for example, an inorganic salt.
25 The two reservoirs 562 and 566 are separated by the impermeable membrane 564,
which is impermeable to the contents of both reservoirs 562 and 566. The reservoir
566 is also connected to another reservoir 568 which contains, for example, an
aqueous solution in which the organic salt is at least partially soluble. The two
30 reservoirs 566 and 568 are separated by a rigid, semi-permeable membrane 570,
20 which is partially or completely impermeable to the salt in reservoir 566 and
partially or fully permeable to the solution in reservoir 568. There is also an
optional fill port or vent 572 in communication with the reservoir 568, through
35 which material can be added to or removed from the reservoir 568. Using this
device 560, water can be drawn from the reservoir 568 across the semi-permeable
25 membrane 570 into the reservoir 566 due to osmosis caused by the presence of salt
in the reservoir 566. The flow of water will cause the volume of reservoir 566 to
40 increase and thereby force the volume of reservoir 562 to decrease, which causes
material to expel from reservoir 562 through microneedles 514.

45 In an alternate embodiment, delivery is initiated by opening the pathway
30 between the reservoir and the microneedle tip, or unblocking the tip openings, and
simply allowing the drug to be delivered by diffusion, that is, a passive process.

(iv). Controlling the Delivery Rate

The microneedle device must be capable of transporting drug across or into

the tissue at a useful rate. For example, the microneedle device must be capable of delivering drug at a rate sufficient to be therapeutically useful. The rate of delivery of the drug composition can be controlled by altering one or more of several design variables. For example, the amount of material flowing through the needles can be controlled by manipulating the effective hydrodynamic conductivity (the volumetric through-capacity) of a single device array, for example, by using more or fewer microneedles, by increasing or decreasing the number or diameter of the bores in the microneedles, or by filling at least some of the microneedle bores with a diffusion-limiting material. It is preferred, however, to simplify the manufacturing process by limiting the needle design to two or three "sizes" of microneedle arrays to accommodate, for example small, medium, and large volumetric flows, for which the delivery rate is controlled by other means.

Other means for controlling the rate of delivery include varying the driving force applied to the drug composition in the reservoir. For example, in passive diffusion systems, the concentration of drug in the reservoir can be increased to increase the rate of mass transfer. In active systems, for example, the pressure applied to the reservoir can be varied, such as by varying the spring constant or number of springs or elastic bands.

In either active or passive systems, the barrier material can be selected to provide a particular rate of diffusion for the drug molecules being delivered through the barrier at the needle inlet.

(v). Feedback about Delivery

In a preferred embodiment, the microneedle device includes a feedback means so that the user can (1) determine whether delivery has been initiated; and/or (2) confirm that the reservoir has been emptied, that is delivery complete. Representative feedback means include a sound, a color (change) indicator, or a change in the shape of a deformable reservoir. In a preferred embodiment, the feedback for completion of delivery is simply that the reservoir is pressed flat against the back of the substrate and cannot be further deformed.

(vi). Feedback about Penetration of Microneedles into Tissue

The user of the microneedle device typically can determine if the microneedles have been properly inserted into the skin or other tissue through visual or tactile means, that is assessing whether the substrate has been pressed essentially

flush to the tissue surface. For example, if a puddle of liquid drug composition appears near the device, then the user may infer that the microneedles are not fully inserted, suggesting that the device needs to be reapplied. The liquid drug compositions can include a coloring agent to enhance the visual feedback.

In a more complex embodiment, an electrical or chemical measurement is adapted to provide the feedback. For example, penetration can be determined by measuring a change in electrical resistance at the skin or other tissue, or a pH change. Alternately, needle-to-needle electrical resistance can be measured. In a preferred embodiment, the microneedle device includes a disposable cartridge containing the microneedles. In these devices, an LED (e.g. green light/red light) or liquid crystal display can be provided with the reusable portion of the device.

(vii). Multi-Cartridge Microneedle Device

A modification of the disposable, single use microneedle device utilizes a reusable triggering device (e.g., a plunger) in combination with a cartridge containing one or more, preferably a plurality, of single-use microneedle devices. For example, the cartridge can be a circular disk having 10 or 12 microneedle arrays connected to a single-dose reservoir, wherein the cartridge can be loaded into and unloaded from the triggering device. The triggering device can, for example, be designed to move a new dose into position for delivery, compress the reservoir to deliver the drug, and then eject or immobilize the used array. This type of reusable triggering device also can include a power source, such as a battery, used to operate a built-in measurement device, for example, for analyte measurement of interstitial fluids or electrical verification of needle penetration into skin.

(viii). Microneedle Device Packaging

In a preferred embodiment following manufacture of the microneedle device, it is packaged for storage, shipment, and sale before use. The packaging should prevent contamination and damage. The packaging also should prevent premature triggering or release of any drug or vehicle contents from the reservoir.

It is particularly important that, the microneedle device is provided with a removable protective cover or cushion that protects the microneedles from damage. The protective cover also can function to keep the drug material from prematurely leaking out of the microneedles. In a preferred embodiment, an adhesive material or gel film used to selectively secure the cover over the microneedles. In an alternate

5 embodiment, the film is antiseptic, and following removal can serve as a wipe to prepare the skin surface before insertion of the microneedles.

10 The packaging also can be adapted to serve as a vessel for safely disposing of the used microneedle device. In a preferred embodiment, the single-use
5 microneedles are provided a device or material to shear the needles from the substrate or plug the microneedles, so as to prevent undesirable reuse of the device. In one embodiment, the inner back of the reservoir is provided with a tacky
15 substance. When the reservoir is compressed against the back of the substrate following delivery of the reservoir contents, the tacky substance is driven into the opening of the microneedles, plugging them. In one embodiment of this device, the
20 tacky material dries and hardens so that the substance cannot readily be removed.

20 b. Diagnostic Sensing of Body Fluids (Biosensors)

The device is applied to the skin or other biological barrier at the site where the sample is to be collected or measured. Then, biological fluid, or a component
25 thereof, is drawn into or through the pores or bores of the microneedles, and optionally collected in the collection chamber. Alternatively, where the microneedles function as the sensor, sensing occurs without transfer of biological fluid into a collection chamber. One embodiment of the devices described herein
30 may be used to remove material from the body across a biological barrier, i.e. for minimally invasive diagnostic sensing. For example, fluids can be transported from interstitial fluid in a tissue into a reservoir in the upper portion of the device. The
35 fluid can then be assayed while in the reservoir or the fluid can be removed from the reservoir to be assayed, for diagnostic or other purposes. For example, interstitial fluids can be removed from the epidermis across the stratum corneum to assay for
25 glucose concentration, which should be useful in aiding diabetics in determining their required insulin dose.

40 The sensing device can be in or attached to one or more microneedles, or in a housing adapted to the substrate. Sensing information or signals can be transferred optically (e.g., refractive index) or electrically (e.g., measuring changes in electrical
45 impedance, resistance, current, voltage, or combination thereof). For example, it may be useful to measure a change as a function of change in resistance of tissue to an electrical current or voltage, or a change in response to channel binding or other

5 criteria (such as an optical change) wherein different resistances are calibrated to
signal that more or less flow of drug is needed, or that delivery has been completed.

10 In one embodiment, one or more microneedle devices can be used for (1)
withdrawal of interstitial fluid, (2) assay of the fluid, and/or (3) delivery of the
5 appropriate amount of a therapeutic agent based on the results of the assay, either
automatically or with human intervention. For example, a sensor delivery system
may be combined to form, for example, a system which withdraws bodily fluid.
15 measures its glucose content, and delivers an appropriate amount of insulin. The
sensing or delivery step also can be performed using conventional techniques, which
10 would be integrated into use of the microneedle device. For example, the
microneedle device could be used to withdraw and assay glucose, and a
20 conventional syringe and needle used to administer the insulin, or *vice versa*.

In an alternate embodiment, microneedles may be purposefully sheared off
from the substrate after penetrating the biological barrier, as described above. The
25 portion of the microneedles which remain within or on the other side of the
biological barrier could contain one or more biosensors. For example, the sensor
could change color as its output. For microneedles sheared off in the skin, this color
change could be observed through the skin by visual inspection or with the aid of an
30 optical apparatus.

20 The microneedles can also be used for aerosolization or delivery for example
directly to a mucosal surface in the nasal or buccal regions or to the pulmonary
system.

35 The microneedle devices disclosed herein also should be useful for
controlling transport across tissues other than skin. For example, microneedles can
25 be inserted into the eye across, for example, conjunctiva, sclera, and/or cornea, to
facilitate delivery of drugs into the eye. Similarly, microneedles inserted into the
40 eye can facilitate transport of fluid out of the eye, which may be of benefit for
treatment of glaucoma. Microneedles may also be inserted into the buccal (oral),
nasal, vaginal, or other accessible mucosa to facilitate transport into, out of, or
45 across those tissues. For example, a drug may be delivered across the buccal
mucosa for local treatment in the mouth or for systemic uptake and delivery. As
30 another example, microneedle devices may be used internally within the body on,
for example, the lining of the gastrointestinal tract to facilitate uptake of

5 orally-ingested drugs or the lining of blood vessels to facilitate penetration of drugs
into the vessel wall. For example, cardiovascular applications include using
microneedle devices to facilitate vessel distension or immobilization, similarly to a
10 stent, wherein the microneedles/substrate can function as a "staple-like" device to
5 penetrate into different tissue segments and hold their relative positions for a period
of time to permit tissue regeneration. This application could be particularly useful
with biodegradable devices. These uses may involve invasive procedures to
15 introduce the microneedle devices into the body or could involve swallowing,
inhaling, injecting or otherwise introducing the devices in a non-invasive or
10 minimally-invasive manner.

20 *(i). Biological Fluids for Withdrawal and Sensing*

The microneedle devices are useful in the transport of biological fluids from
within or across a variety of biological barriers including the skin (or parts thereof):
the blood-brain barrier; mucosal tissue; blood vessels; lymphatic vessels; cell
25 membranes; epithelial tissue; and endothelial tissue. The biological barriers can be
in humans or other types of animals, as well as in plants, insects, or other organisms,
including bacteria, yeast, fungi, and embryos. In preferred embodiments, biological
fluids are withdrawn from skin, more preferably human skin, for minimally invasive
30 diagnostic sensing.

20 Biological fluids useful with the devices described herein include blood,
lymph, interstitial fluid, and intracellular fluid. A preferred biological fluid to be
withdrawn or sensed is interstitial fluid.

35 A variety of analytes are routinely measured in the blood, lymph or other
body fluids. Examples of typical analytes that can be measured include blood sugar
25 (glucose), cholesterol, bilirubin, creatine, various metabolic enzymes, hemoglobin,
heparin, hematocrit, vitamin K or other clotting factors, uric acid, carcinoembryonic
40 antigen or other tumor antigens, and various reproductive hormones such as those
associated with ovulation or pregnancy. Other substances or properties desirable to
detect include lactate (important for athletes), oxygen, pH, alcohol, tobacco
45 30 metabolites, and illegal drugs (important for both medical diagnosis and law
enforcement).

In a preferred embodiment, interstitial fluids are removed from the dermis or
epidermis across the stratum corneum to assay for glucose concentration, which is

5 useful in aiding diabetics in determining their required insulin dose.

(ii). Feedback about Microneedle Penetration into Tissue

10 The user of the microneedle device typically can determine if the microneedles have been properly inserted into the skin or other tissue through visual or tactile means, that is assessing whether the substrate has been pressed essentially flush to the tissue surface. A coloring agent can be used to enhance the visual feedback by indicating a color change triggered by biological fluid filling the collection chamber.

15 In a more complex embodiment, an electrical or chemical measurement is adapted to provide the feedback. For example, penetration can be determined by measuring a change in electrical resistance at the skin or other tissue, or a pH change. Alternately, needle-to-needle electrical resistance can be measured. In a preferred embodiment, the microneedle device includes a disposable cartridge containing the microneedles. In these devices, an LED (e.g., green light/red light) or liquid crystal display can be provided with the reusable portion or the device.

25 (iii). Feedback about Withdrawal

In a preferred embodiment, the microneedle device includes a feedback means so that the user can determine whether withdrawal and/or sensing has been completed. Representative feedback means include a sound, a color (change) indicator, or a change in the position or shape of a reservoir or collection chamber.

30 (iv). Initiating and Controlling Fluid Withdrawal

35 In a preferred embodiment, the microneedle device is capable of transporting molecules across or from the tissue at a useful rate. That rate will, of course, depend on the particular application. For assaying blood glucose, for example, the device preferably withdraws at least between about 5 and 10 μ l of interstitial fluid, preferably in about a minute or less time. For other applications, it may be desirable to apply the device to the barrier for several hours or more in order to monitor the changing blood plasma level of a particular analyte, such as an exogenous drug or hormone level, for example on a real-time basis or to obtain a time-averaged value.

40 The rate of withdrawal can be controlled by altering one or more of several design variables. For example, the amount of material flowing through the needles can be controlled by manipulating the volumetric through-capacity of a single device array, e.g., by using more or fewer microneedles, by increasing or decreasing the

5 number or diameter of the bores in the microneedles, by filling at least some of the
microneedle bores with a diffusion-limiting material, or by varying the driving force
10 applied to the biological fluid. It is preferred, however, to simplify the
manufacturing process by limiting the needle design to two or three "sizes" of
5 microneedle arrays to accommodate, for example small, medium, and large
volumetric flows, for which the withdrawal rate is controlled by other means.

15 The flow of biological fluid from the tissue through the microneedle and into
the collection chamber or into contact with the sensors occurs due to capillary
action, diffusion, or is induced using conventional mechanical pumps or
10 nonmechanical driving forces, such as electroosmosis or electrophoresis, thermal
gradients, or convection. For example, in electroosmosis, electrodes are positioned
20 on the biological barrier surface, on one or more microneedles, and/or on the
substrate adjacent the needles, to create a convective flow which carries charged
ionic species and/or neutral molecules toward and/or through at least one of the
25 microneedles.

Transportation of molecules through the microneedles can be controlled or
monitored using, for example, various combinations of semi-permeable membranes,
valves, pumps, sensors, actuators, and microprocessors. These components can be
30 produced using standard manufacturing or microfabrication techniques. Actuators
20 that may be useful with the microneedle devices disclosed herein include
micropumps, microvalves, and positioners.

35 In preferred embodiments, the microneedle device is used with another
mechanism that enhances the permeability of the biological barrier, such as by
increasing cell membrane disruption, using electric fields, ultrasound, chemical
25 enhancers, vacuum, viruses, pH, heat, and/or light. Chemical and/or physical
enhancers can be applied to the biological barrier at the insertion site of the device
40 before or during the withdrawal of the device, for example, to draw analyte closer to
the skin surface.

(a). bulk flow extraction

45 30 A preferred microneedle device is shown in Figure 26 and described above.
Microneedle device 620 preferably is operated as follows. After or simultaneously
with the insertion of device 620 into, for example, the skin, manual pressure is
50 applied to elastic cap 622 so as to deform (compress) it and reduce the interior

5 volume of elastic cap 622 and fluid collection chamber 616. The deformation
causes gas within the cap and chamber to be purged from the device via one-way
valve 624. As elastic cap 622 returns to its undeformed (uncompressed) shape,
10 pressure is reduced within the interior volume, creating a pressure differential or
vacuum, which causes the interstitial fluid, to be drawn through the microneedles
5 614 and into fluid collection chamber 616, until the pressure is equalized. Once in
the collection chamber 616, the fluid sample can be analyzed by withdrawing device
15 620 from the skin, again depressing elastic cap 622, to force the sample out of the
chamber either through the microneedles 614 or one-way valve 624, and, for
10 example, onto a diagnostic strip or into a container adapted for the particular
analytical method to be employed.

20 Other spring means can be adapted to cause a change in the volume, and thus
internal pressure, of the collection chamber. For example, the fluid collection
chamber can be adapted to have a movable, rigid top with fixed, rigid side walls,
25 wherein the interface between the walls and top form a gas-tight seal (such as by
15 using a gasket). The volume of the piston-like apparatus can be expanding by
activating one or more compressed springs to move the top of the chamber as
desired, thereby reducing the pressure in the collection chamber.

30 In an alternative embodiment, withdrawal can be initiated by activating an
osmotic pump, as described, for example, in U.S. Patent No. 4,320,758 to
20 Eckenhoff, which has been engineered to create a volume expansion/pressure
reduction in the collection chamber to draw biological fluid to be drawn into the
35 collection chamber.

40 In a preferred embodiment, withdrawal is conducted using a microneedle
25 device fitted to a Luer-Lock syringe or similar conventionally-used devices that
currently uses hypodermic needles in the barrier penetration method.

(b). diffusion-based extraction

45 One preferred embodiment uses diffusion to move the analyte fluid into the
fluid collection chamber. A microneedle device using this method generally
30 includes microneedle bores or pores, and/or a fluid collection chamber, that are
filled with a diffusion medium, such as water, a saline solution, or a gel, which is
physiologically compatible with the biological barrier tissue. Once the needle is
50 inserted into the biological barrier (e.g., the skin), the diffusion medium contacts the

5 biological fluid. Typically, the diffusion medium in the microneedles initially
contains none of the analyte to be measured; therefore, analyte at a higher
concentration in the biological fluid diffuses into the diffusion medium in the
10 microneedle until a detectable level of analyte is collected or measured. This should
5 be achieved rapidly due to the very small size/length of the microneedles, thereby
providing an analyte concentration for sensing that is rapidly response to that in the
tissue.

15 (c). hybrid bulk flow/diffusion

In another embodiment, the microneedle device is designed to employ a
10 combination of forces to drive the analyte into the collection chamber. A preferred
hybrid design includes the preferred bulk flow microneedle device described above,
20 but with two primary differences. First, the fluid collection chamber has no one-way
valve and contains a fluid diffusion medium, preferably physiological saline.
Second, a temporary barrier is interposed between the fluid collection chamber and
25 the base of the microneedles. The temporary barrier can be a fracturable membrane,
mechanical gate, or other means for containing the diffusion medium within the
device until the barrier is broken or removed at a selected time to permit flow of
molecules between the microneedles and fluid collection chamber.

30 In a preferred embodiment, the temporary barrier is an easily fracturable
membrane. The device can function as follows: The microneedles first are inserted
20 into the skin of the user. Then the user depresses the elastic cap, causing the fluid
diffusion medium to fracture the membrane and fill the bores or pores of the
35 microneedles and contact the biological fluid. After the user releases the elastic cap,
it partially or fully returns to its undeformed shape, reducing the pressure in the
interior and causing a mixture of the biological fluid and diffusion medium to be
25 drawn through the microneedles and into fluid collection chamber. Once bulk fluid
40 flow ceases, diffusion may continue until the concentration of biological fluid or
analyte equilibrates. The mixture can be assayed as described herein, considering
the dilution effect induced by the presence of the diffusion medium.

45 30 Any of these embodiments of the microneedle device can be adapted to
function a series of micro-assays (e.g., as can be provided with an electronics
package) or single assays (e.g., standard glucose strips).

5

(v). Multi-Cartridge Microneedle Device

10

A modification of the disposable, single use microneedle device utilizes a reusable portion providing the withdrawal force (e.g., suction) or electronics package in combination with a cartridge containing one or more, preferably a plurality, of single-use, disposable microneedle devices for collection and/or sensing. For example, the cartridge can be a circular disk having 10 or 12 microneedle arrays connected to a single-assay element, wherein the cartridge can be loaded into and unloaded from the reusable portion. The triggering device can, for example, be designed to move a new microneedle array into position, withdraw or sense the sample of biological fluid, and then eject or immobilize the used microneedle array. This type of reusable triggering device also can include a power source, such as a battery, used to operate a built-in measurement device, for example, for analyte measurement of interstitial fluids. In one embodiment, the devices are provided in a multipack (e.g., six or twelve pack) form of complete devices, that is, each device is fully sufficient for use. Individual devices can be separated as needed for each sensing measurement.

15

10

20

25

c. Delivery of Energy

30

Other than transport of drugs and biological molecules, the microneedles may be used to transmit or transfer other materials and energy forms, such as light, electricity, heat, or pressure. The microneedles, for example, could be used to direct light to specific locations within the body, in order that the light can directly act on a tissue or on an intermediary, such as light-sensitive molecules in photodynamic therapy.

35

The present invention will be further understood with reference to the following non-limiting examples.

Example 1: Fabrication of Solid Silicon Microneedles

40

45

A chromium masking material was deposited onto silicon wafers and patterned into dots having a diameter approximately equal to the base of the desired microneedles. The wafers were then loaded into a reactive ion etcher and subjected to a carefully controlled plasma based on fluorine/oxygen chemistries to etch very deep, high aspect ratio valleys into the silicon. Those regions protected by the metal mask remain and form the microneedles.

30

50

55

5 <100>-oriented, prime grade, 450-550 μm thick, 10-15 $\Omega\text{-cm}$ silicon wafers
(Nova Electronic Materials Inc., Richardson, TX) were used as the starting material.
The wafers were cleaned in a solution of 5 parts by volume deionized water, 1 part
10 30% hydrogen peroxide, and 1 part 30% ammonium hydroxide (J.T. Baker,
5 Phillipsburg, NJ) at approximately 80°C for 15 minutes, and then dried in an oven
(Blue M Electric, Watertown, WI) at 150°C for 10 minutes. Approximately 1000 Å
15 of chromium (Mat-Vac Technology, Flagler Beach, FL) was deposited onto the
wafers using a DC-sputterer (601 Sputtering System, CVC Products, Rochester,
NY). The chromium layer was patterned into 20 by 20 arrays of 80 μm diameter
10 dots with 150 μm center-to-center spacing using the lithographic process described
20 below.

A layer of photosensitive material (1827 photoresist, Shipley, Marlborough,
MA) was deposited onto the chromium layer covering the silicon wafers. A
standard lithographic mask (Telic, Santa Monica, CA) bearing the appropriate dot
25 array pattern was positioned on top of the photoresist layer. The wafer and
photoresist were then exposed to ultraviolet (UV) light through the mask by means
of an optical mask aligner (Hybralign Series 500, Optical Associates, Inc., Milpitas,
CA). The exposed photoresist was removed by soaking the wafers in a liquid
30 developer (354 developer, Shipley, Marlborough, MA) leaving the desired dot array
20 of photoresist on the chromium layer. Subsequently, the wafers were dipped into a
chromium etchant (CR-75; Cyantec, Fremont, CA), which etched the chromium
that had been exposed during the photolithography step, leaving dot arrays of
35 chromium (covered with photoresist) on the surface of the silicon wafer. The
photoresist still present on the chromium dots formed the masks needed for
25 fabrication of the microneedles, described below.

40 The microneedles were fabricated using a reactive ion etching techniques
based on the Black Silicon Method developed at the University of Twente. The
patterned wafers were etched in a reactive ion etcher (700 series wafer/batch Plasma
Processing System, Plasma Therm, St. Petersburg, FL) with means for ensuring
45 good thermal contact between the wafers and the underlying platen (Apiezon N, K.J.
Lesker, Clairton, PA). The wafers were etched using the following gases and
conditions: SF_6 (20 standard cubic centimeters per minute) and O_2 (15 standard
50 cubic centimeters per minute) at a pressure of 150 mTorr and a power of 150 W for
63

5 a run time of approximately 250 minutes. These conditions caused both deep
vertical etching and slight lateral underetching. By controlling the ratio of flow rates
of the SF₆ and O₂ gases used to form the plasma, the aspect ratio of the microneedles
10 could be adjusted. The regions protected by the chromium masks remained and
5 formed the microneedles. Etching was allowed to proceed until the masks fell off
due to underetching, resulting in an array of sharp silicon spikes.

Example 2: Transdermal Transport Using Solid Microneedles

15 To determine if microfabricated microneedles could be used to enhance
transdermal drug delivery, arrays of microneedles were made using a deep plasma
10 etching technique. Their ability to penetrate human skin without breaking was
tested and the resulting changes in transdermal transport were measured.

20 Arrays of microneedles were fabricated having extremely sharp tips (radius
of curvature less than 1 μm), and are approximately 150 μm long. Because the skin
surface is not flat due to dermatoglyphics and hair, the full length of these
25 microneedles will not penetrate the skin. All experiments were performed at room
temperature (23±2 °C).

30 The ability of the microneedles to pierce skin without breaking was then
tested. Insertion of the arrays into skin required only gentle pushing. Inspection by
light and electron microscopy showed that more than 95% of microneedles within an
20 array pierced across the stratum corneum of the epidermis samples. Moreover,
essentially all of the microneedles that penetrated the epidermis remained intact. On
those very few which broke, only the top 5-10 μm was damaged. Microneedle
35 arrays could also be removed without difficulty or additional damage, as well as re-
inserted into skin multiple times.

25 To quantitatively assess the ability of microneedles to increase transdermal
transport, calcein permeability of human epidermis with and without inserted
microneedle arrays was measured. Calcein crosses skin very poorly under normal
40 circumstances and therefore represents an especially difficult compound to deliver.
As expected, passive permeability of calcein across unaltered skin was very low.
45 indicating that the epidermis samples were intact.

30 Insertion of microneedles into skin was capable of dramatically increasing
permeability to calcein. When microneedles were inserted and left embedded in the
skin, calcein permeability was increased by more than 1000-fold. Insertion of
50

microneedles for 10 s, followed by their removal, yielded an almost 10,000-fold increase. Finally, insertion of a microneedle array for 1 h, followed by its removal, increased skin permeability by about 25,000-fold. Permeabilities for skin with microneedles inserted and then removed are higher than for skin with microneedles remaining embedded probably because the microneedles themselves or the silicon plate supporting the array may block access to the microscopic holes created in the skin. Light microscopy showed that the holes which remained in the skin after microneedles were removed were approximately 1 μm in size.

To confirm *in vitro* experiments which showed that skin permeability can be significantly increased by microneedles, studies were conducted with human volunteers. They indicated that microneedles could be easily inserted into the skin of the forearm or hand. Moreover, insertion of microneedle arrays was never reported to be painful, but sometimes elicited a mild "wearing" sensation described as a weak pressure or the feeling of a piece of tape affixed to the skin. Although transport experiments were not performed *in vivo*, skin electrical resistance was measured before and after microneedle insertion. Microneedles caused a 50-fold drop in skin resistance, a drop similar to that caused by the insertion of a 30-gauge "macroneedle." Inspection of the site immediately after microneedle insertion showed no holes visible by light microscopy. No erythema, edema, or other reaction to microneedles was observed over the hours and days which followed. This indicates that microneedle arrays can permeabilize skin in human subjects in a non-painful and safe manner.

Example 3: Fabrication of Silicon Microtubes

Three-dimensional arrays of microtubes were fabricated from silicon, using deep reactive ion etching combined with a modified black silicon process in a conventional reactive ion etcher. The fabrication process is illustrated in Figures 4a-d. First, arrays of 40 μm diameter circular holes 32 were patterned through photoresist 34 into a 1 μm thick SiO_2 layer 36 on a two inch silicon wafer 38 (Figure 4a). The wafer 38 was then etched using deep reactive ion etching (DRIE) (Laermer, et al., "Bosch Deep Silicon Etching: Improving Uniformity and Etch Rate for Advanced MEMS Applications," *Micro Electro Mechanical Systems*, Orlando, Florida, USA (Jan. 17-21, 1999)), in an inductively coupled plasma (ICP) reactor to etch deep vertical holes 40. The deep silicon etch was stopped after the holes 40 are

5 approximately 200 μm deep into the silicon substrate 38 (Figure 4b) and the photoresist 34 was removed. A second photolithography step patterned the remaining SiO_2 layer 36 into circles concentric to the holes, thus leaving ring shaped
10 oxide masks 34 surrounding the holes (Figure 4c). The photoresist 34 was then removed and the wafer 38 was again deep silicon etched, while simultaneously the holes 40 were etched completely through the wafer 38 (inside the SiO_2 ring) and the silicon was etched around the SiO_2 ring 38 leaving a cylinder 42 (Figure 4d). The
15 resulting tubes were 150 μm in height, with an outer diameter of 80 μm , an inner diameter of 40 μm , and a tube center-to-center spacing of 300 μm .

10 **Example 4: Micromold Fabrication of Metal Microtubes**

Hollow metal microtubes were prepared without dry silicon etching, using a thick, photo-defined mold of epoxy. The sequences are illustrated in Figures 5a-e. First, a thick layer of SU-8 epoxy 44 was spin cast onto a silicon or glass substrate 46 that had been coated with 30 nm of titanium 48, the sacrificial layer. Arrays of
25 cylindrical holes 49 were then photolithographically defined through an epoxy layer 44, typically 150 μm thick (Figure 5a). The sacrificial layer then was partially removed using a wet etching solution containing hydrofluoric acid and water at the bottom of the cylindrical holes in the SU-8 photoresist 46 (Figure 5b). A seed layer
30 of Ti/Cu/Ir (30 nm/200 nm/30 nm) 39 was then conformally DC sputter-deposited onto the upper surface of the epoxy mold and onto the sidewalls of the cylindrical holes 49 (Figure 5c). As shown in Figure 5c, the seed layer 39 was electrically isolated from the substrate. Subsequently, NiFe was electroplated onto the seed
35 layer 39 (Figure 5d), the epoxy 44 was removed from the substrate, and the surrounding epoxy 44 was removed (Figure 5e). The resulting microtubes are 200 μm in height with an outer diameter of 80 μm , an inner diameter of 60 μm , and a
40 tube center-to-center spacing of 150 μm . The holes in the interior of the microtubes protrude through the base metal supporting the tubes.

Example 5: Micromold Fabrication of Tapered Microneedles

45 A micromold having tapered walls was fabricated by molding a preexisting 3-D array of microneedles, i.e. the mold-insert, and subsequently removing the mold insert. The micromold was then surface plated in a manner similar to that for the

5 microtubes described in Example 4. The fabrication sequence is illustrated in Figures 6a-d.

10 First, an array of solid silicon microneedles 50 were prepared as described in Henry, et al., "Micromachined Needles for the Transdermal Delivery of Drugs,"
5 *Micro Electro Mechanical Systems*, Heidelberg, Germany, Jan. 26-29, pp. 494-98 (1998). Then, a layer of epoxy 52 (SU-8) was spin cast onto the microneedle array to completely blanket the array (Figure 6a). The epoxy 52 settled during pre-bake to
15 create a planar surface above the tips of the microneedles 50. The epoxy 52 was then fully pre-baked, photolithographically cross-linked, and post-baked.

20 Then, the upper surface of the epoxy 52 was etched away using an O_2/CHF_3 plasma until approximately 1 to 2 μm of the needle tips 54 were exposed, protruding from the epoxy 52 (Figure 6b). The silicon was then selectively removed by using a SF_6 plasma (Figure 6c). The remaining epoxy mold 52 provided a negative of the
25 microneedles with a small diameter hole where the tip of the silicon needle protruded. After the removal of the silicon, a seed layer of Ti-Cu-Ti 54 was conformally sputter-deposited onto the top and sidewalls of the epoxy micromold 52. Following the same process sequence as described in Example 4, NiFe was then
30 electroplated onto the seed layer 54 (Figure 6c). Finally, the epoxy was removed using an O_2/CHF_3 plasma, leaving a 20 x 20 array of NiFe hollow metal
35 microneedles 54 (Figure 6d). The microneedles 54 were 150 μm in height with a base diameter of 80 μm , a tip diameter of 10 μm , and a needle-to-needle spacing of 150 μm .

40 Micromold-based microneedles also have been successfully manufactured using a process in which the epoxy mold material was replaced with PDMS. In this
45 case, it was possible to remove the mold from the mold insert, as well as the microneedles from the mold, using only physical techniques such as peeling. This
50 approach advantageously requires no dry etching and allows one to reuse both the mold and the mold insert.

55 **Example 6: Micromold Fabrication of Tapered Microneedles Using Laser-Formed Molds**

A micromold having tapered walls was fabricated by use of laser ablation techniques, as shown in Figures 7a-d. A laser-ablatable polymer sheet 60 such as
65 KAPTONTM polyimide approximately 150 μm in thickness was optionally

5 laminated to a thin (10-30 μm) metal sheet 62 such as titanium (Figure 7a). A
tapered hole 64 was formed in the metal/polymer laminate 60/62 using a laser
10 technique such as excimer laser ablation (Figure 7b). The entry hole of the laser
spot was on the metal side 62, and a through hole was made through both the metal
5 sheet and the polymer film. The through hole 64 was tapered in combination with
either defocusing or appropriate substrate motion to create a taper such that the wide
end of the hole 64 (typically 40-50 μm) was on the metal side 62 and the narrow end
15 of the hole 64 (typically 10-20 μm) was on the polymer 60 side. A thin layer of
metal 66, e.g. titanium, of thickness 0.1 μm was then deposited, e.g., using a sputter-
10 deposition technique, in such a way that the metal 66 deposited on the metal film
side and coated the polymer sidewalls, but did not coat the polymer 60 side of the
laminate (Figure 7c). Electrodeposition of metal 68, e.g., gold, to a thickness of 1 to
20 5 μm was then performed on the titanium-coated metal surface 66, and polymer
sidewalls curved section of 60 next to 64. Finally, the polymer 60 was removed,
25 using e.g. an oxygen plasma, to form the completed microneedles (Figure 7d).

Alternate polymer removal methods, such as thermal, solvent, aqueous, or
photo-degradation followed by solvent or aqueous removal, are also possible if the
30 polymer material is chosen appropriately (e.g., a photoresist resin).

Example 7: Formation of Microneedles by Embossing

20 Formation of a microneedle by embossing is shown in Figures 8a-f. A
polymeric layer 70 (Figure 8a) is embossed by a solid microneedle or microneedle
array 72 (Figure 8b). The array 72 is removed (Figure 8c), and the layer 70 is etched
35 from the non-embossed side 74 until the embossed cavity 76 is exposed (Figure 8d).
A metallic layer 78 is then deposited on the embossed side and the sidewalls, but not
25 on the non-embossed side 74 (Figure 8e). This layer 78 is optionally thickened by
electrodeposition of an additional metal layer 80 on top of it (Figure 8e). The
40 polymer layer 70 is then removed to form the microneedles 78/80 (Figure 8f).

Example 8: Transdermal Application of Hollow Microneedles

45 The bore of hollow microneedles must provide fluid flow with minimal
30 clogging in order to be suitable to transport material, such as in transdermal drug
delivery. Therefore, microneedles and microtubes were evaluated to determine their
suitability for these functions.

5
10
15
Hollow metal and silicon microneedles, produced as described in Examples 3-5, were inserted through human skin epidermis with no apparent clogging of the needle bores. Scanning electron microscopy of a hollow metal (NiFe) microneedle penetrating up through the underside of human epidermis showed the microneedle remains intact, with the tip free of debris. Similarly, silicon microneedles, metal microneedles, and metal microtubes were successfully inserted through human skin. Also, the hollow microneedles were shown to permit the flow of water through their bores.

Example 9: Drug Transport Through Microneedles Inserted Into Skin

10
20
25
15
Studies were performed with solid and hollow microneedles to demonstrate transport of molecules and fluids. As shown in Table 1, transport of a number of different compounds across skin is possible using microneedles. These studies were performed using either solid silicon microneedles or using hollow silicon microneedles made by methods described in this patent. Transport was measured across human cadaver epidermis *in vitro* using Franz diffusion chambers at 37 °C using methods described in Henry, et al., "Microfabricated microneedles: A novel method to increase transdermal drug delivery" *J. Pharm. Sci.* 87: 922-25 (1998).

30
35
25
The transdermal delivery of calcein, insulin, bovine serum albumin ("BSA"), and nanoparticles was measured. Delivery refers to the ability to transport these compounds from the stratum corneum side of the epidermis to the viable epidermis side. This is the direction of transport associated with delivering drugs into the body. Removal of calcein was also measured. Removal refers to the ability to transport calcein from the viable epidermis side of the epidermis to the stratum corneum side. This is the direction of transport associated with removing from the body compounds found in the body, such as glucose.

40
45
30
50
In all cases shown in Table 1, transport of these compounds across skin occurred at levels below the detection limit when no needles were inserted into the skin. Intact skin provides an excellent barrier to transport of these compounds. In all cases examined, when solid microneedles were inserted into the skin and left in place, large skin permeabilities were measured, indicating that the microneedles had created pathways for transport across the skin. Furthermore, in all cases, when solid microneedles were inserted into the skin and then removed, even greater skin permeabilities resulted. Finally, when hollow microneedles were inserted into the

skin and left in place, still greater skin permeabilities resulted for those compounds tested. These studies show that microneedles can dramatically increase skin permeability and can thereby increase transport of a number of different compounds across the skin. They also shows that when solid microneedles are used, a preferred embodiment involves inserting and then removing microneedles, rather than leaving them in place. They also shows that using hollow microneedles are a preferred embodiment over the use of solid microneedles.

Table 1: Transport of Drugs Through Microneedles Inserted Into Skin

Compound	No needles	Solid needles inserted	Solid needles inserted and removed	Hollow needles inserted
Calcein delivery	**	4×10^{-3}	1×10^{-2}	1×10^{-1}
Calcein removal	**	2×10^{-3}	1×10^{-2}	n.a.
Insulin delivery	**	1×10^{-2}	1×10^{-2}	n.a.
BSA delivery	**	9×10^{-3}	8×10^{-2}	9×10^{-2}
Nanoparticle delivery	**	n.a.	3×10^{-2}	n.a.

** means that the transport was below the detection limit.

n.a. means that the data are not available.

Nanoparticles were made of latex with a diameter of approximately 100 nm.

Example 10: Flow of Water Through Hollow Microneedles

To demonstrate that fluid can be forced through hollow microneedles at meaningful rates, the flow rate of water through a microneedle array was measured as a function of pressure. The array used contained 100 hollow silicon microneedles having an inner diameter of 50 μm and an outer diameter of 80 μm . The results, which are shown in Table 2, demonstrate that significant flow rates of water through microneedles can be achieved at modest pressures. The measured flow rates are comparable to flow rates through hypodermic needles attached to syringes.

Table 2: Flow Rate of Water Through Hollow Silicon Microneedles as a Function of Applied Pressure

Pressure (psi)	Flow rate (ml/min)
1.0	16
1.5	24
2.0	31
2.5	38
3.0	45

5

Modifications and variations of the methods and devices described herein will be obvious to those skilled in the art from the foregoing detailed description. Such modifications and variations are intended to come within the scope of the appended claims.

10

15

20

25

30

35

40

45

50

55

Claims

5

10

15

20

25

30

35

40

45

50

55

5

We claim:

10

1. A device for transport of a material across or into a biological barrier comprising

a) a plurality of hollow microneedles each having a base end and a tip, with at least one hollow pathway disposed at or between the base end and the tip,

b) a substrate to which the base ends of the microneedles are attached or integrated, and

15

c) at least one reservoir which is in connection with the base ends of at least one of the microneedles, either integrally or separably until the moment of use,

wherein the volume or amount of material to be transported can selectively be altered.

20

2. The device of claim 1 wherein the reservoir is formed of a material which is deformable.

3. The device of claim 2 wherein the reservoir is elastic.

25

4. The device of claim 1 wherein the reservoir further comprises a therapeutic, prophylactic, or diagnostic agent.

5. The device of claim 4 wherein the agent is selected from the group consisting of peptides, proteins, carbohydrates, nucleic acid molecules, lipids, organic molecules, biologically active inorganic molecules, and combinations thereof.

30

6. The device of claim 1 further comprising a plunger movably secured to the substrate, wherein the plunger can compress the reservoir.

35

7. The device of claim 6 further comprising a spring engaged with the plunger.

8. The device of claim 1 wherein the diameter of the microneedles is between about 10 μm and about 200 μm .

40

9. The device of claim 1 wherein the length of the microneedles is between about 100 μm and 1 mm.

10. The device of claim 1 wherein the microneedles are adapted to provide an insertion depth of less than about 100 to 150 μm .

45

11. The device of claim 1 comprising a three dimensional array of microneedles.

12. The device of claim 1 further comprising an adhesive material for

50

55

5 securing the device during delivery.

13. The device of claim 1 wherein the reservoir is a syringe or pump
connected to the substrate.

10 14. The device of claim 1 comprising an attachment means for securing the
device to a syringe or pump.

15 15. The device of claim 13 wherein the substrate is adapted to removably
connect to a standard or Luer-lock syringe.

16. The device of claim 1 further comprising a sealing mechanism which is
interposed between the reservoir and the substrate or which is secured to the tips of
the microneedles.

20 17. The device of claim 16 wherein the sealing mechanism is a fracturable
barrier interposed between the reservoir and the substrate.

18. The device of claim 1 further comprising a means for providing
feedback to indicate that delivery has been initiated or completed.

25 19. The device of claim 1 wherein at least the microneedles are
manufactured for single use as a disposable reagent.

20. The device of claim 1 wherein the device further comprises means for
stopping delivery.

30 21. The device of claim 1 further comprising an osmotic pump to move
agent.

22. The device of claim 1 wherein the microneedle is at an angle other than
perpendicular to the substrate.

35 23. The device of claim 1 wherein the substrate is formed of a flexible
material.

24. The device of claim 1 comprising multiple compartments or reservoirs.

40 25. The device of claim 24 wherein the compartments or reservoirs can be
connected or in communication with each other.

26. The device of claim 24 wherein one or more reservoirs contain a solid
formulation and one or more reservoirs contains a liquid carrier for the solid
formulation.

45 27. The device of claim 1 in a packaging that protects the device from
damage and/or contamination.

50 28. The device of claim 1 further comprising a removable liner that covers

5

the microneedle tips and that can be used to protect and/or seal access to or from the microneedles.

10

29. The device of claim 1 wherein the device comprises rate control means, which can be used to regulate the rate or extent at which materials flow through the microneedles.

15

30. The device of claim 29 wherein the rate control means is a membrane at one end of the microneedles through which agent or fluid must pass.

31. The device of claim 29 wherein the rate control means is a material positioned within the hollow pathway of the microneedles.

20

32. The device of claim 1 comprising multiple microneedle arrays in combination with means for accessing one or more arrays at a time.

33. The device of claim 1 comprising means for preventing undesired contact with or use of the microneedles.

25

34. The device of claim 33 wherein the means is packaging that covers the microneedles.

35. The device of claim 33 wherein the means is packaging that shears off the microneedles, or tips thereof, after use.

30

36. The device of claim 33 wherein the means are materials which are delivered into the hollow pathways to seal the microneedles.

37. A method for delivering a therapeutic, prophylactic or diagnostic agent across or into tissue comprising

35

inserting into the tissue one or more microneedles that are in fluid connection with at least one reservoir containing the agent to be delivered, and

reducing the volume or amount of the agent in the reservoir by driving the agent through at least one of the microneedles.

40

38. The method of claim 37 wherein the reservoir is formed of a material which is deformable.

39. The method of claim 37 wherein the volume or amount of the agent in the reservoir is reduced by depressing a plunger that is movably secured to the substrate.

45

40. A kit of parts for delivering a therapeutic, prophylactic or diagnostic agent across or into tissue comprising

50

(a) one or more microneedle devices which comprise a plurality of hollow

55

5 microneedles, a substrate to the microneedles are attached or integrated, and at least
one reservoir which is selectably in communication with the microneedles, wherein
at least one of the reservoirs contains the therapeutic, prophylactic or diagnostic
10 agent to be delivered; and

(b) a triggering device which is adapted to activate delivery of the agent
from reservoir through the microneedles of one of the devices at a time.

41. A device for collecting a sample of a biological fluid comprising:

15 (a) one or more hollow or porous microneedles having a base end and a tip,

(b) a substrate to which the base of the microneedle is attached or integrated,

and

20 (c) at least one collection chamber which is selectably in fluid
communication with the base end of the microneedle.

42. The device of claim 41 further comprising

25 (d) a means for inducing transport of the biological fluid or component
thereof into the collection chamber.

43. The device of claim 42 wherein the pressure within the collection
chamber can selectively be reduced.

30 44. The device of claim 43 wherein the pressure reduction is induced by
expanding the internal volume of the collection chamber.

45. The device of claim 44 wherein the collection chamber is a standard or
Luer-lock syringe.

35 46. The device of claim 43 wherein the collection chamber comprises an
upper portion which is formed of a material which is deformable.

47. The device of claim 43 further comprising a plunger movably secured to
the substrate, wherein the plunger can deform the collection chamber.

40 48. The device of claim 46 further comprising a one-way valve.

49. The device of claim 41 wherein the collection chamber comprises a
plurality of compartments.

45 50. The device of claim 41 comprising a three dimensional array of
microneedles.

51. The device of claim 41 further comprising an adhesive material for
securing the device to the biological barrier surface during fluid withdrawal or
50 sensing.

5

52. The device of claim 41 further comprising a means for controlling flow through the microneedle.

10

53. The device of claim 42 wherein the means for controlling flow is a fracturable or removable barrier which is interposed between the collection chamber and base of the microneedle.

15

54. The device of claim 41 further comprising a sensor in communication with the collection chamber.

55. A device for sensing an analyte in a biological fluid, the device comprising:

20

(a) one or more microneedles having a base end and a tip,

(b) a substrate to which the base of the microneedle is attached or integrated,

(c) at least one sensor which is selectably in communication with the microneedle.

25

56. The device of claim 55 wherein the sensor comprises a chemical or biochemical agent that react with the analyte, and electrochemical or optical transducers which measure the reaction of the agent and analyte.

30

57. The device of claim 56 wherein the agent is an enzyme selected from the group consisting of glucose oxidase, glucose dehydrogenase, and combinations thereof.

35

58. The device of claim 55 further comprising an electronics package in communication with the sensor.

59. The device of claim 55 for insertion of the microneedles in skin and sensing of glucose.

40

60. A device for sensing an analyte in a biological fluid, the device comprising:

(a) one or more microneedles having a base end and a tip,

(b) a substrate to which the base of the microneedle is attached or integrated, wherein at least one of the microneedles is or comprises a sensor.

45

61. The device of claim 60 wherein the sensor comprises a chemical or biochemical agent that react with the analyte, and electrochemical or optical transducers which measure the reaction of the agent and analyte.

50

55

5

62. The device of claim 60 further comprising an electronics package in communication with the sensor.

10

63. The device of claim 60 for insertion of the microneedles in skin and sensing of glucose.

64. The device of claim 41 wherein the collection chamber is adapted to receive and use glucose strips.

15

65. The device of claim 41 wherein the microneedle is hollow and comprises at least one opening in the side of the microneedle.

20

66. The device of claim 41 wherein the microneedle has a hollow bore containing a material to modulate the flow of biological fluid through the microneedles into the collection chamber.

67. A method for collecting a sample of a biological fluid or analyte therein, comprising the steps:

25

providing a device comprising (i) one or more hollow or porous microneedles having a base end and a tip, (ii) a substrate to which the base of the microneedle is attached or integrated, (iii) at least one collection chamber which is selectably in fluid connection with the base end of the microneedle, and (iv) a means for inducing transport of the biological fluid or component thereof into the collection chamber;

30

inserting the microneedles into a biological barrier comprising biological fluid; and

35

triggering the induction means to permit the transport of the biological fluid or a component thereof through the microneedles and into the collection chamber.

68. The method of claim 67 wherein the induction means is selected from capillary action, diffusion, mechanical pumps, electroosmosis, electrophoresis, convection, and combinations thereof.

40

69. The method of claim 67 wherein the induction means utilizes a pressure gradient in which the pressure within the microneedles and/or collection chamber is less than the pressure of the biological fluid adjacent the tip of the microneedle.

45

70. The method of claim 67 wherein the analyte to be collected or sensed is selected from the group consisting of glucose, cholesterol, bilirubin, creatine, metabolic enzymes, hemoglobin, heparin, clotting factors, uric acid, tumor antigens, reproductive hormones, oxygen, pH, alcohol, tobacco metabolites, and illegal drugs.

50

55

5

71. A method sensing an analyte in a biological fluid, comprising the steps:

10

(a) providing a device comprising (i) one or more hollow or porous microneedles having a base end and a tip, (ii) a substrate to which the base of the microneedle is attached or integrated, and (iii) at least one sensor which is in communication with one or more of the microneedles;

15

(b) inserting the microneedles into a biological barrier comprising biological fluid; and

(c) contacting the sensor with the biological fluid.

20

72. The method of claim 71 wherein the device further comprises (iv) at least one collection chamber which is selectably in fluid connection with the base end of the microneedle, and (v) a means for inducing transport of the biological fluid or component thereof into the collection chamber, and

25

wherein, after step (b), the induction means is triggered to draw the biological fluid or a component thereof through the microneedles and into the collection chamber.

30

73. The method of claim 72 wherein the induction means utilizes a pressure gradient in which the pressure within the microneedles and/or collection chamber is less than the pressure of the biological fluid adjacent the tip of the microneedle.

74. The method of claim 73 wherein the pressure gradient is created by increasing the volume within the collection chamber.

35

75. The method of claim 71 wherein the analyte to be collected or sensed is selected from the group consisting of glucose, cholesterol, bilirubin, creatine, metabolic enzymes, hemoglobin, heparin, clotting factors, uric acid, tumor antigens, reproductive hormones, oxygen, pH, alcohol, tobacco metabolites, and illegal drugs.

40

76. The method of claim 27 or 31 for sensing glucose wherein the biological barrier is human skin.

45

77. A device for transport of material or energy across or into an elastic biological barrier comprising

a microneedle having a tip end and a base end,

a substrate connected to the base end of the microneedle, and

a means for improving penetration of the biological barrier by the microneedle.

50

55

5

78. The device of claim 77 wherein the biological barrier is human or other mammalian skin.

10

79. The device of claim 77 wherein the means comprises one or more extensions (i) interposed between the substrate and the base end of the microneedle or (ii) extending from the side of the substrate distal to the base end of the microneedle.

15

80. The device of claim 79 wherein the extension is between about 500 μm and about 10 mm in height.

81. The device of claim 79 wherein the extension has a cross-sectional dimension of at least about 200 μm .

20

82. The device of claim 79 wherein the extension includes an array of microneedles extending therefrom.

83. The device of claim 79 wherein the extension is composed of a material which is different from the material forming the microneedles.

25

84. The device of claim 79 wherein the microneedle is hollow and wherein the extension includes at least one aperture in communication with the bore of the microneedle.

30

85. The device of claim 79 further comprising a rigid surface positioned apart from an array of the microneedles and oriented to contact an elastic biological barrier substantially at the same time as the microneedles when the microneedles are applied to the barrier.

35

86. The device of claim 77 wherein the substrate is curved.

87. The device of claim 77 comprising a plurality of microneedles of varying lengths.

40

88. The device of claim 87 comprising four or more microneedles wherein the tip ends of the microneedles collectively define a curvilinear surface.

45

89. The device of claim 77 comprising a plurality of hollow microneedles in a linear array, wherein the substrate is mounted on a holder having one or more apertures through the holder in communication with the microneedles.

90. The device of claim 77 wherein the substrate is flexible.

91. The device of claim 90 wherein the substrate is deformable by fluid pressure or mechanical means.

50

55

5

92. The device of claim 91 wherein the substrate is mounted onto a flexible membrane bubble.

10

93. The device of claim 92 further comprising a second membrane bubble positioned to define a chamber between the flexible membrane bubble and the second membrane bubble.

15

94. The device of claim 93 wherein the chamber contains molecules which flow through the microneedle.

95. The device of claim 94 wherein the molecules are drug molecules.

96. The device of claim 77 wherein the means reduces the elasticity of the biological barrier.

20

97. The device of claim 96 wherein the means physically manipulates the biological barrier to present a more rigid surface in the area of the biological barrier to be penetrated by the microneedle.

25

98. The device of claim 97 wherein the manipulation is selected from the group consisting of stretching, pulling, pinching, and a combination thereof.

99. The device of claim 98 wherein the manipulation includes pulling by reducing the atmospheric pressure over the area of the biological barrier to be penetrated by the microneedles.

30

100. The device of claim 99 further comprising a body portion defining a first vacuum region and a second vacuum region.

wherein an array of microneedles separates the first and second regions.

35

101. The device of claim 100 wherein the body portion comprises an annular ring which holds the microneedles.

40

102. The device of claim 101 wherein the microneedle is hollow and wherein the body portion further comprises a means for attachment to a syringe, a conduit for connection to a vacuum pump, or both.

103. The device of claim 98 wherein the means for physically manipulating comprises a stretching cone or expandable ring around the microneedles.

45

104. The device of claim 98 wherein the means comprises a body portion from which a plurality of stretching elements are pivotally attached.

105. The device of claim 104 wherein the stretching elements have ends provided with a non-slip feature for engagement with the biological barrier.

50

106. The device of claim 98 wherein the means comprises jaws for pinching

55

5 a portion of the biological barrier for contact with the microneedles.

107. The device of claim 97 wherein the means comprises an adhesive film applied over the area of the biological barrier to be penetrated by the microneedle.

108. The device of claim 79 wherein the means for improving penetration creates holes in the stratum corneum, wherein the microneedle can be inserted into the holes.

109. The device of claim 108 wherein the means for creating holes is selected from the group consisting of thermal ablation, high pressure fluid puncturing, cryoablation, and application of degradation agents.

110. The device of claim 77 wherein the means for improving penetration accelerates the tips of the microneedles into the biological barrier, accelerates the biological barrier into contact with the tips of the microneedles, or a combination thereof.

111. The device of claim 110 wherein the means for accelerating the tip of the microneedle comprises releasing a spring or gas under compression.

112. The device of claim 77 wherein a lubricating material is incorporated into or coated onto the microneedle.

113. The device of claim 77 further comprising a collar to limit the depth of microneedle penetration.

114. The device of claim 77 further comprising a means for attaching the device to the skin of a patient, wherein the means is not the microneedle.

115. The device of claim 114 wherein the means is an adhesive film.

116. The device of claim 114 wherein the means is an arm band.

117. The device of claim 77 wherein the microneedle is hollow and wherein the device further comprises a reservoir selectably in communication with the hollow microneedle.

118. The device of claim 77 wherein the means for enhancing penetration comprises an apparatus for vibrating the microneedle.

119. The device of claim 118 wherein the apparatus comprises a piezoelectric transducer or an electromechanical actuator.

120. A kit of parts for use in transport of material or energy across or into an elastic biological barrier, comprising

(i) a device comprising one or more microneedles having a tip end and a

5

base end, and a substrate connected to the base end of the microneedle, and

(ii) an adhesive film or barrier-tightening chemical, either of which can be applied over an area of the biological barrier to be penetrated by the microneedle.

10

121. A method for transport of material or energy across or into an elastic biological barrier comprising using the device of any of claims 77-119.

122. The device of any of claims 1-36 and 41-66 further comprising a means for improving penetration of the biological barrier by the microneedles.

15

20

25

30

35

40

45

50

55

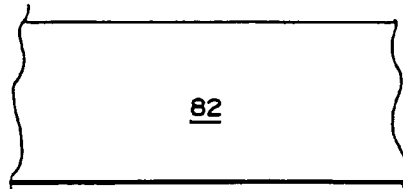


FIG. 1A

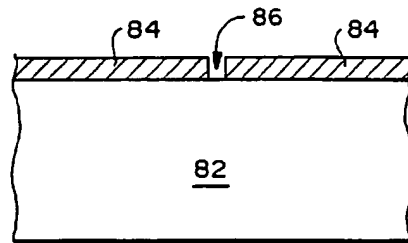


FIG. 1B

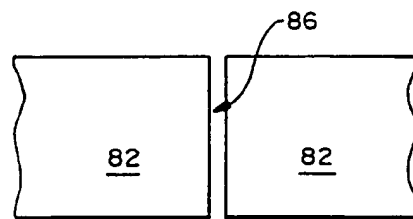


FIG. 1C

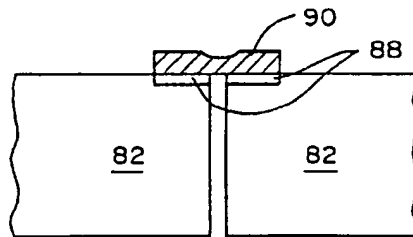


FIG. 1D

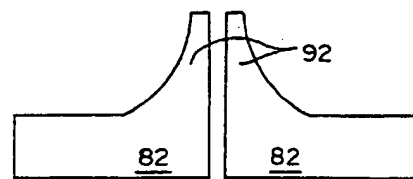


FIG. 1E

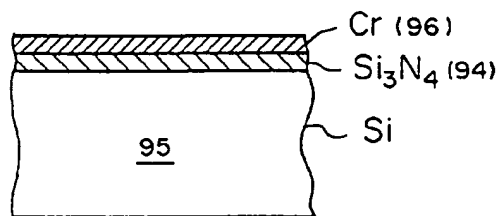


FIG. 2A

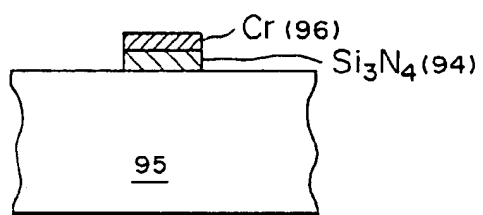


FIG. 2B

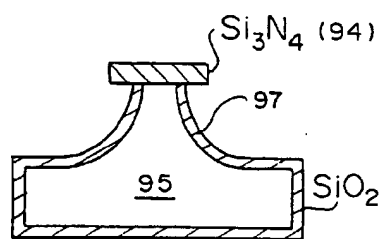


FIG. 2E

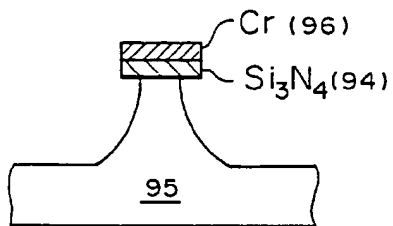


FIG. 2C

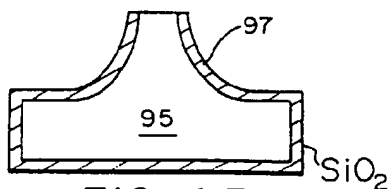


FIG. 2F

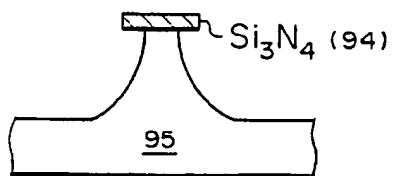


FIG. 2D

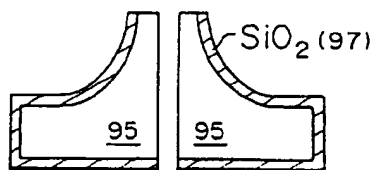


FIG. 2G

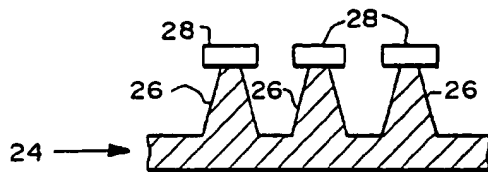


FIG. 3A

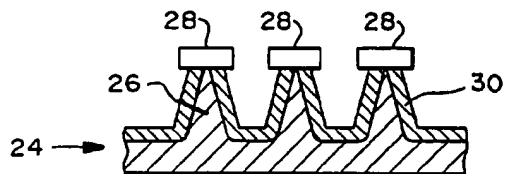


FIG. 3B

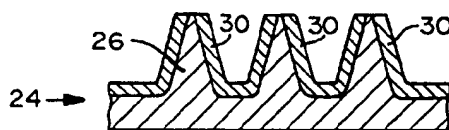


FIG. 3C




FIG. 3D

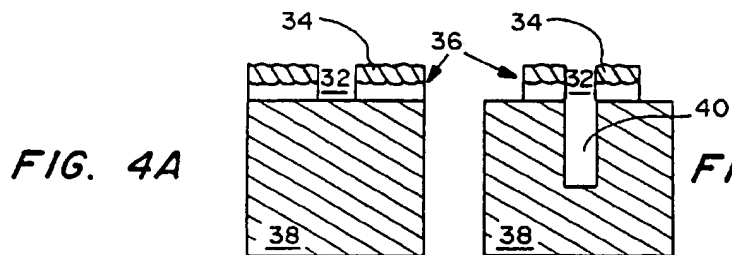


FIG. 4A

FIG. 4C

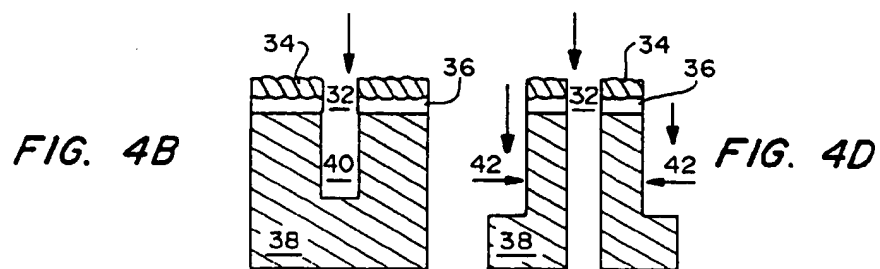
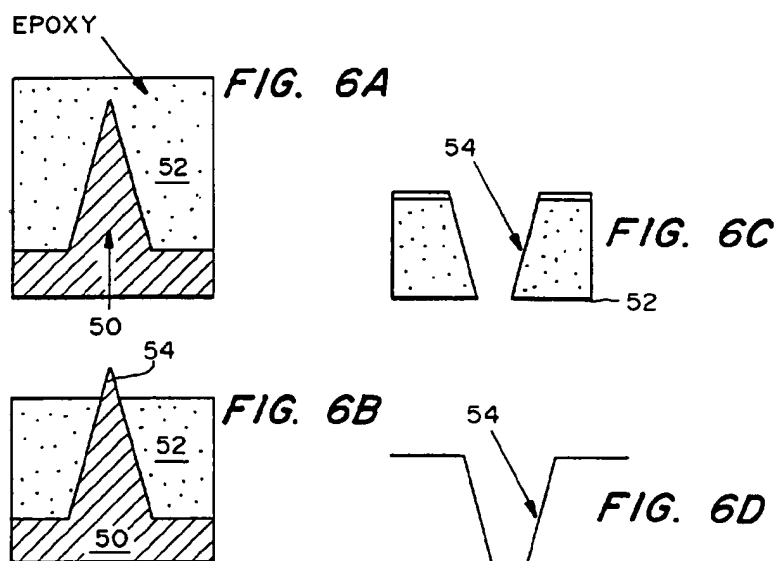
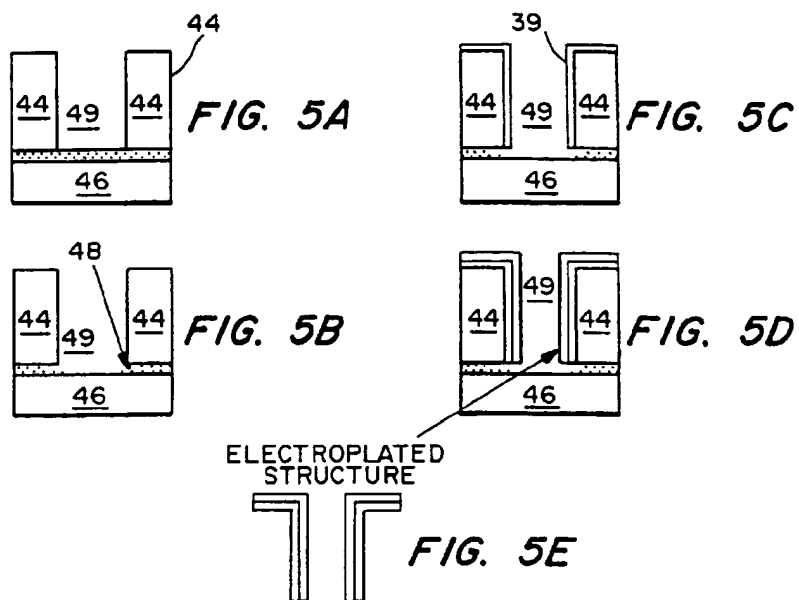


FIG. 4B

FIG. 4D



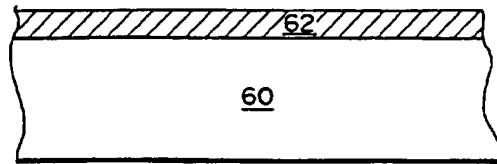


FIG. 7A

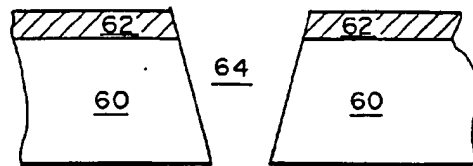


FIG. 7B

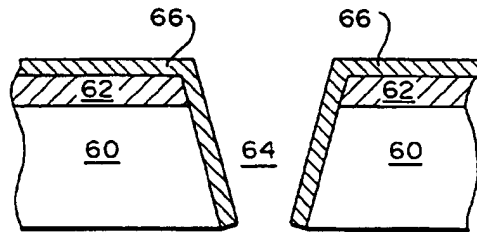


FIG. 7C

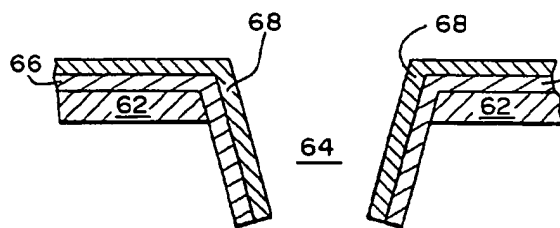


FIG. 7D

6/19

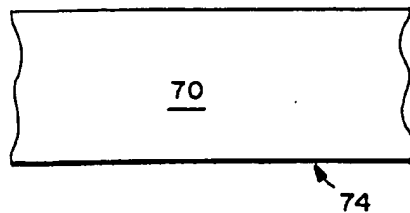


FIG. 8A

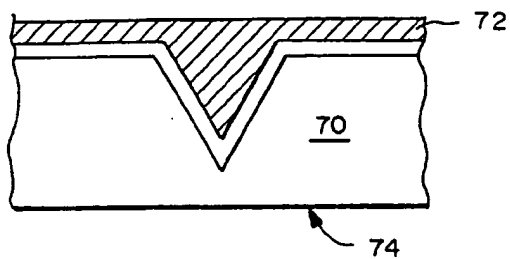


FIG. 8B

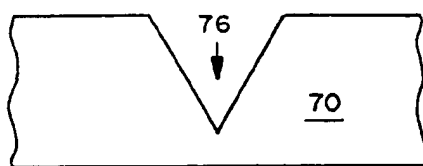


FIG. 8C

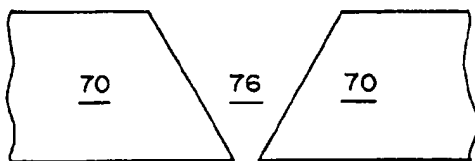


FIG. 8D





FIG. 8E





FIG. 8F

7/19

FIG. 9

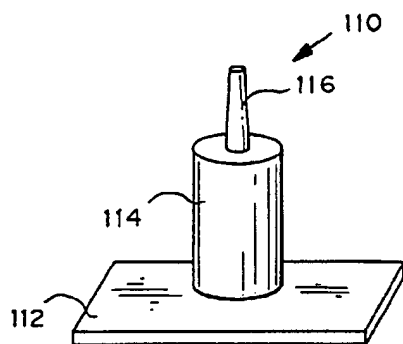
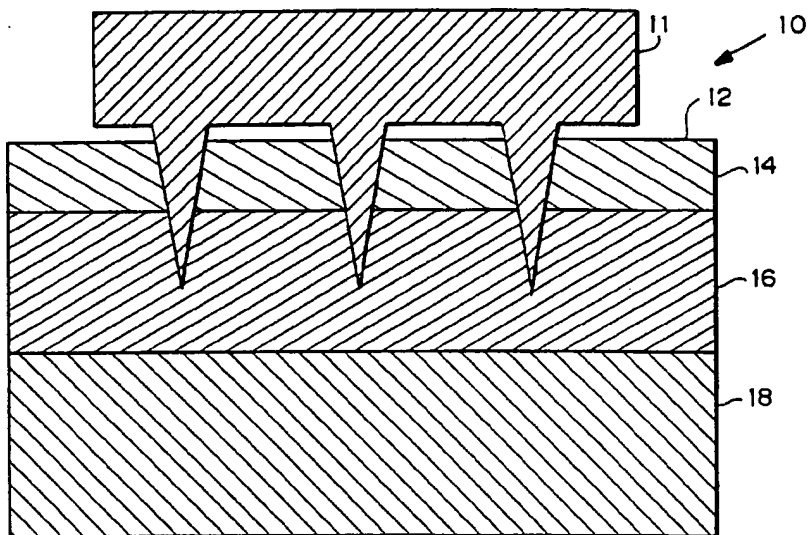


FIG. 10A

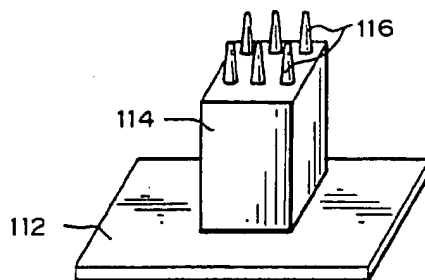


FIG. 10B

8/19

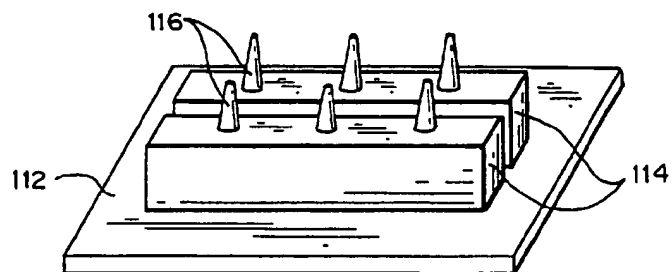


FIG. 10C

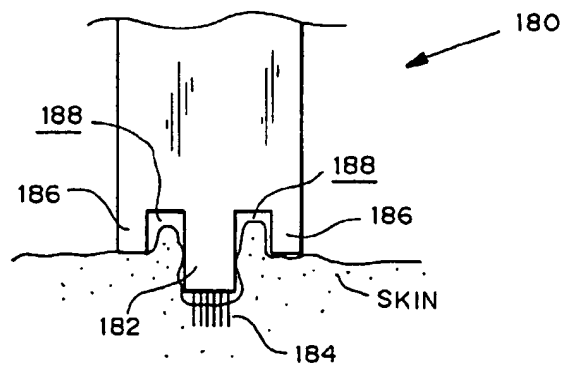


FIG. 10D

FIG. 11A

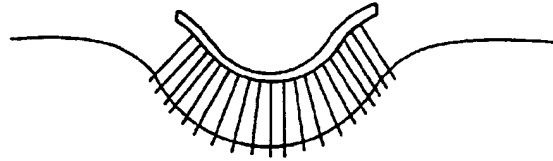


FIG. 11B


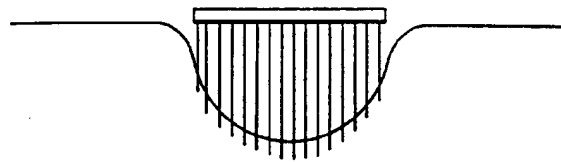


FIG. 11C

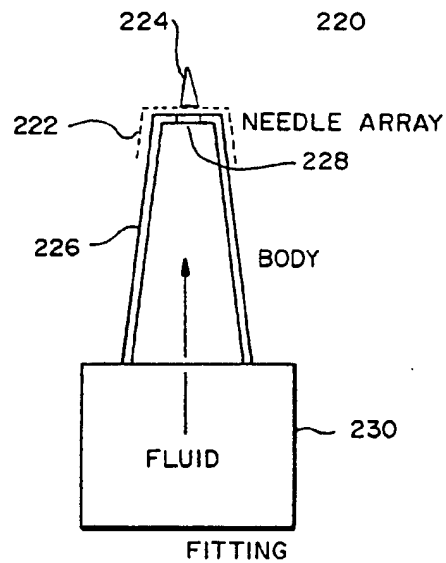

10/19

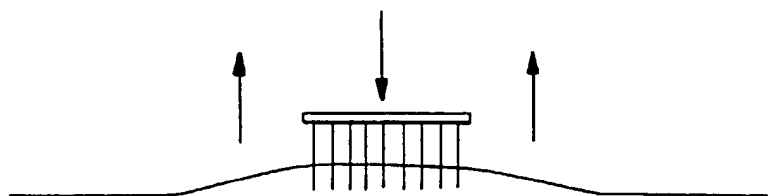


FIG. 12A




FIG. 12B








FIG. 12C

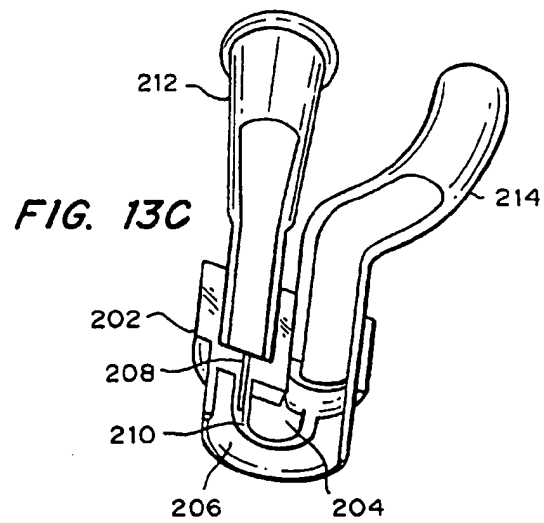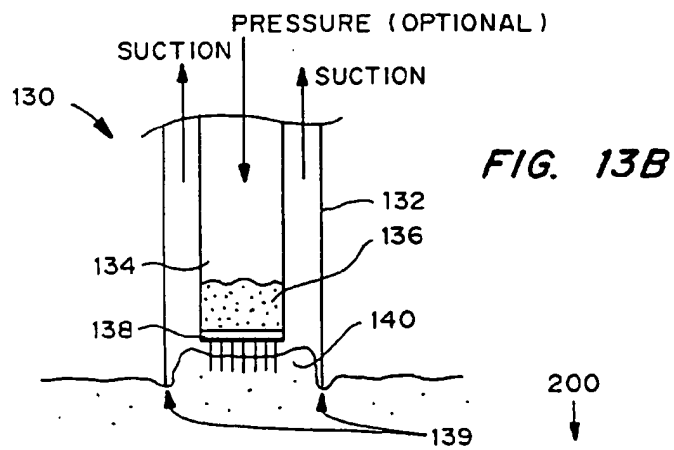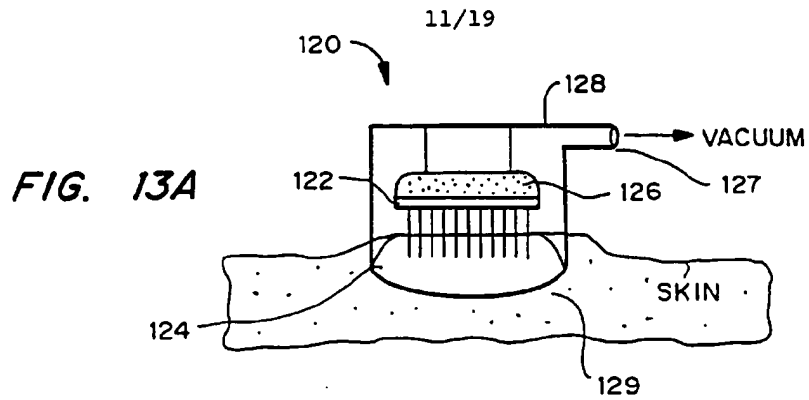

12/19
DEVICE RESTING ON SKIN SURFACE

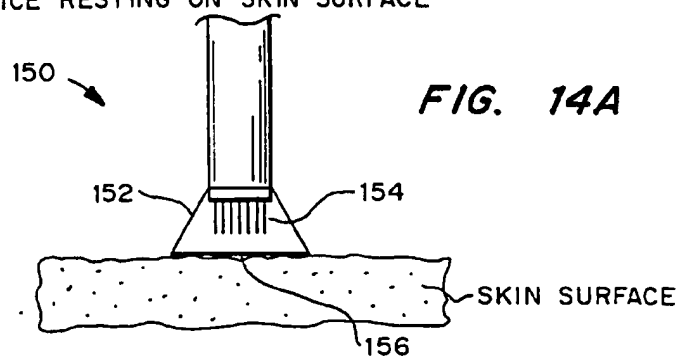

FORCE APPLIED TO MICRONEEDLE / STRETCHING DEVICE


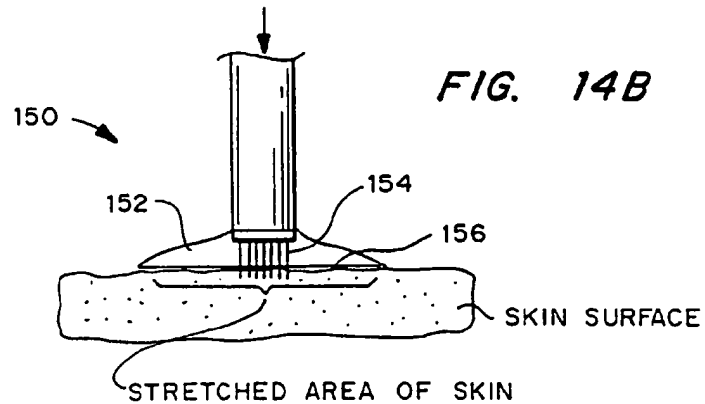


FIG. 14C

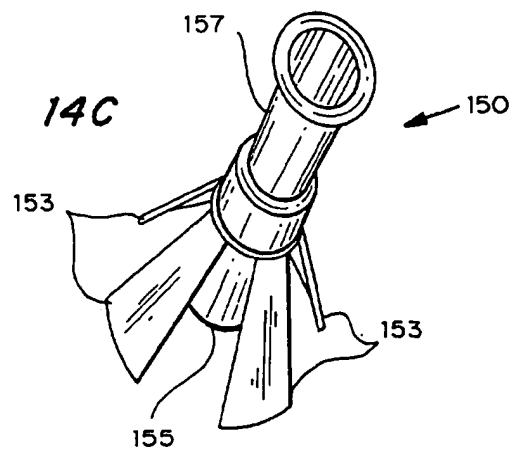

13/19

DEVICE RESTING ON SKIN SURFACE - JAWS OPEN

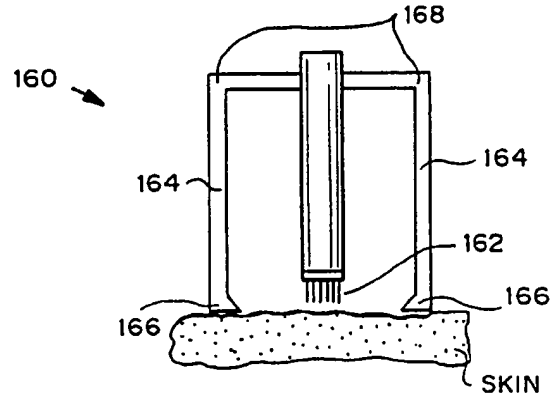


FIG. 15A

DEVICE PINCHING SKIN - JAWS CLOSED

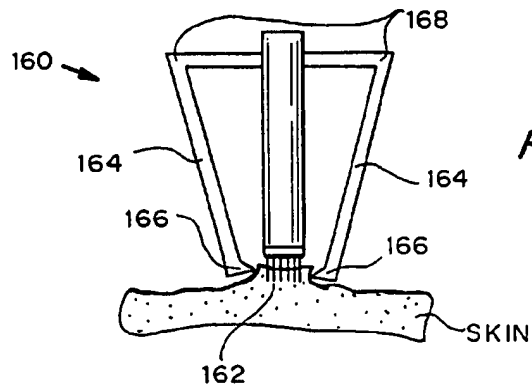


FIG. 15B

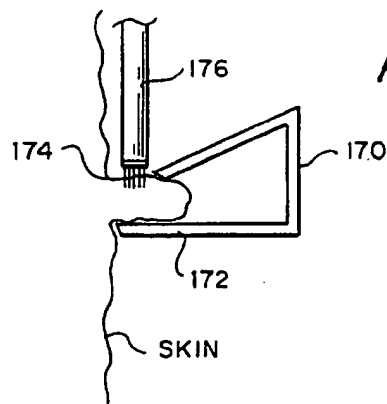


FIG. 15C

14/19

FIG. 16

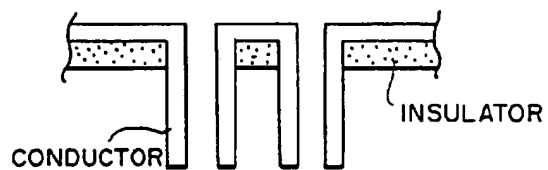


FIG. 17

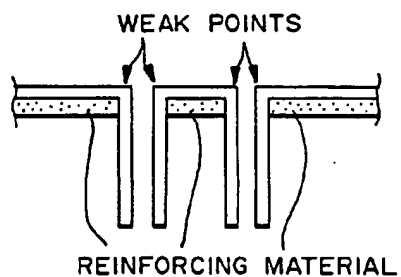


FIG. 18A






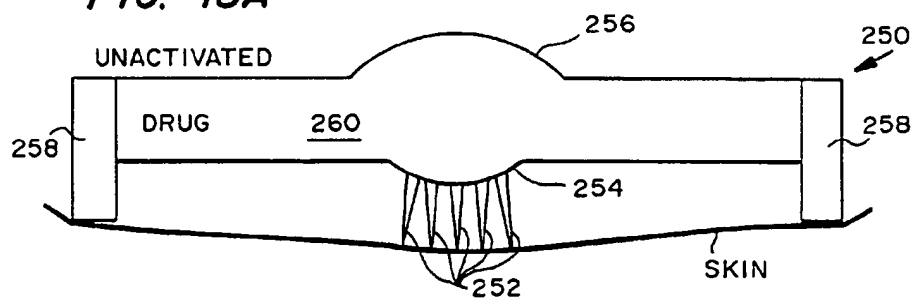


FIG. 18B

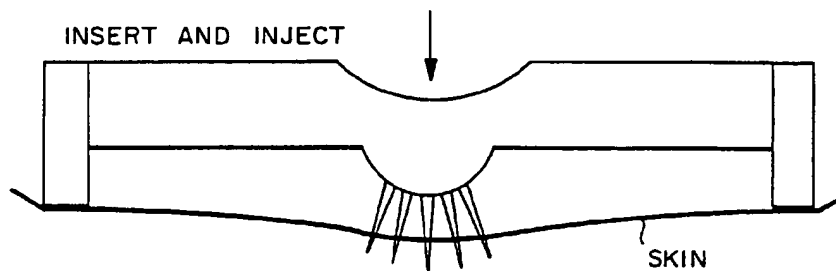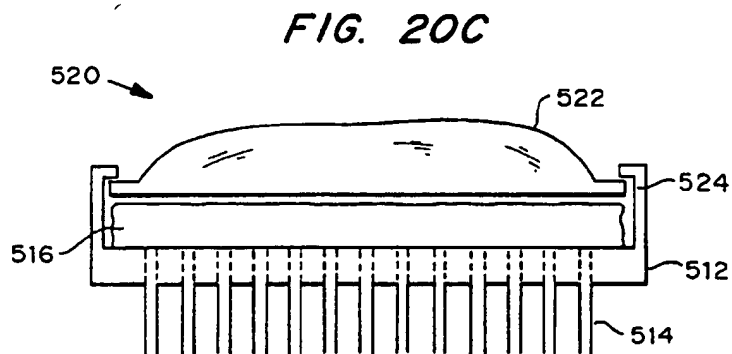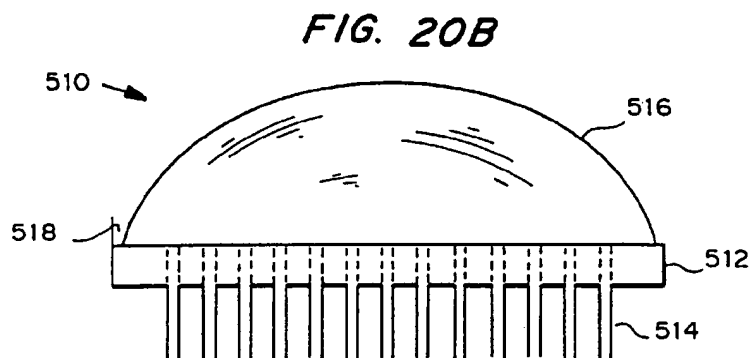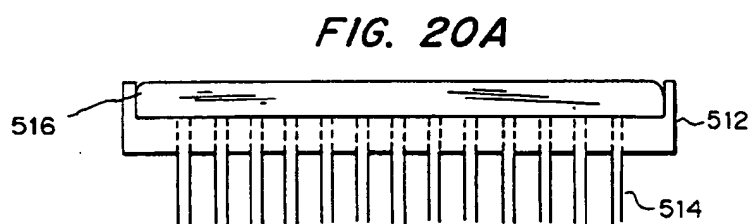

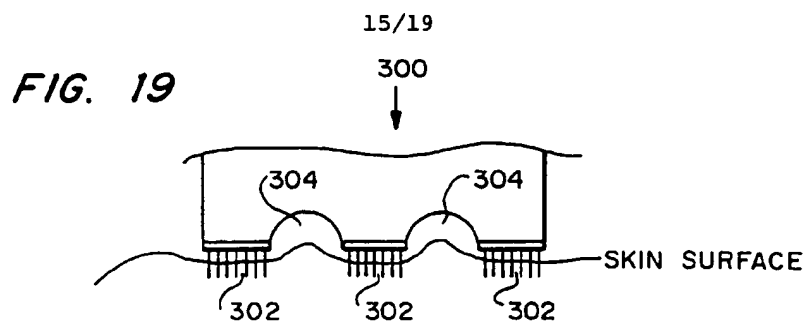

16/19

FIG. 21

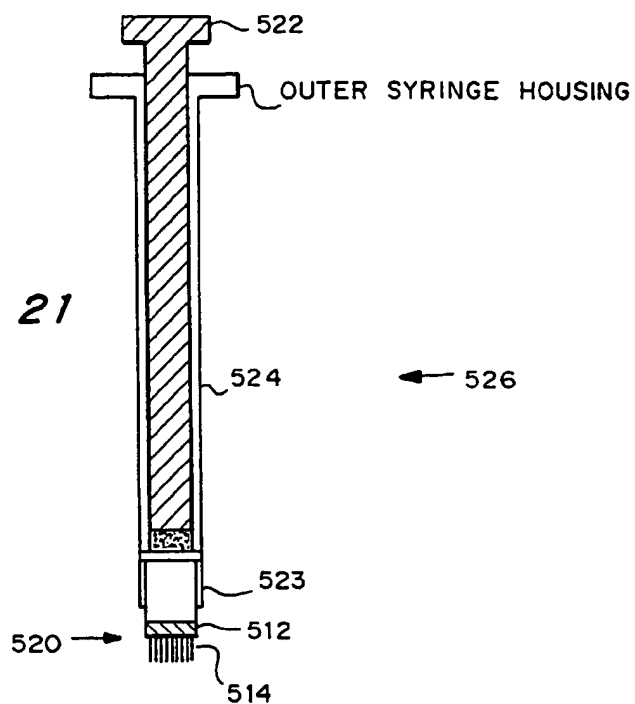
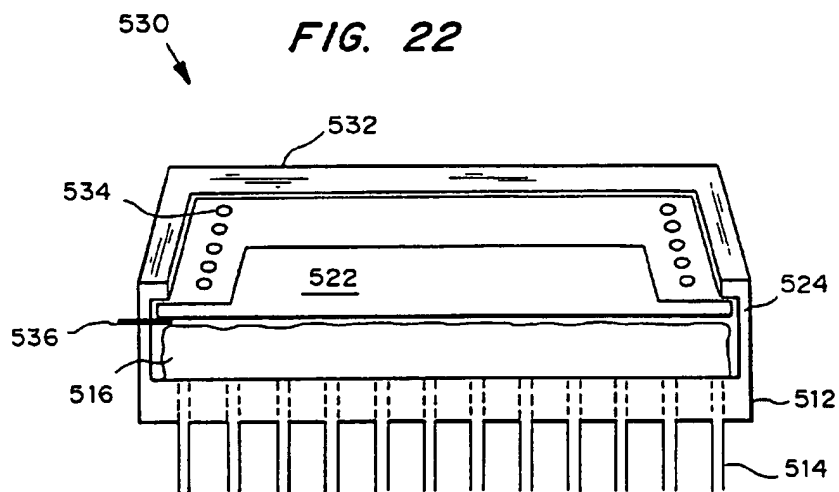


FIG. 22



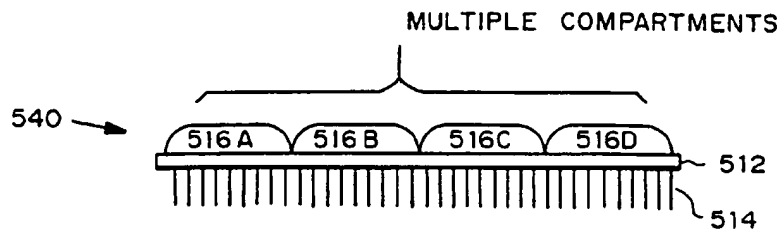


FIG. 23A

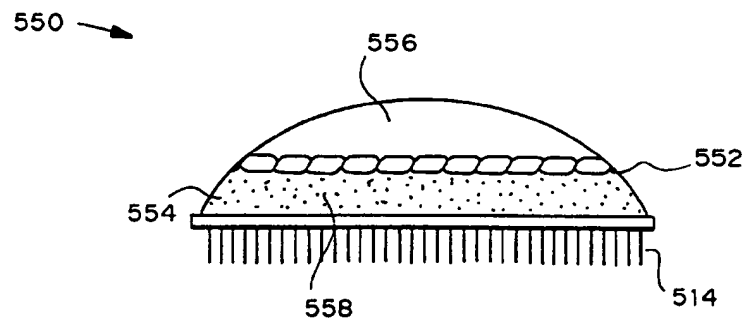
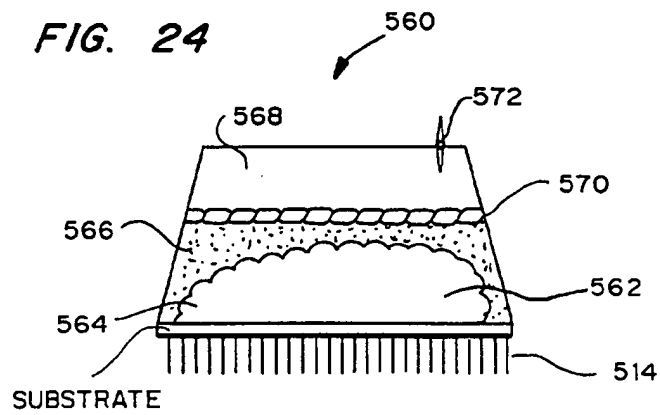
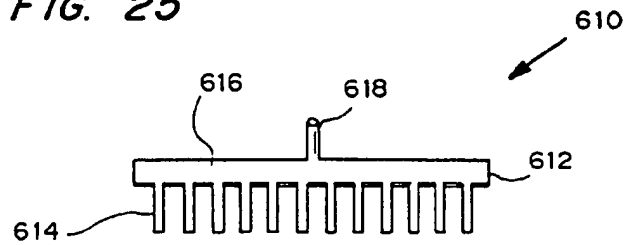
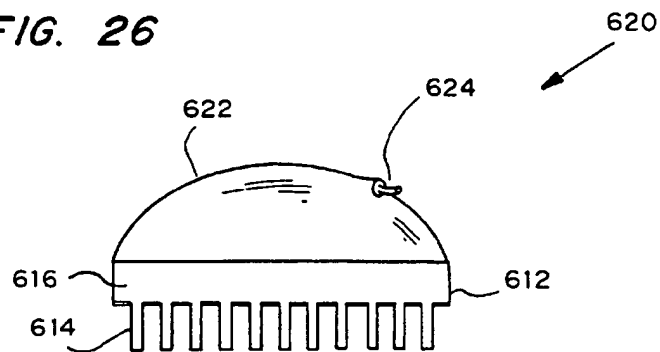


FIG. 23B

18/19

FIG. 24**FIG. 25****FIG. 26**

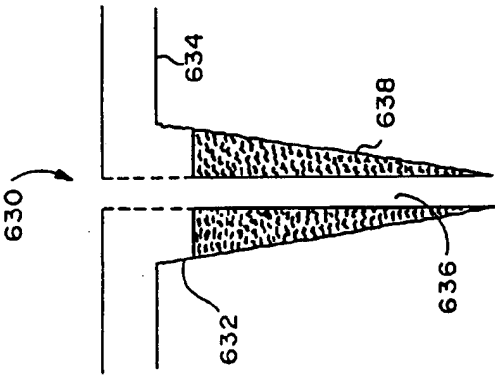


FIG. 27C

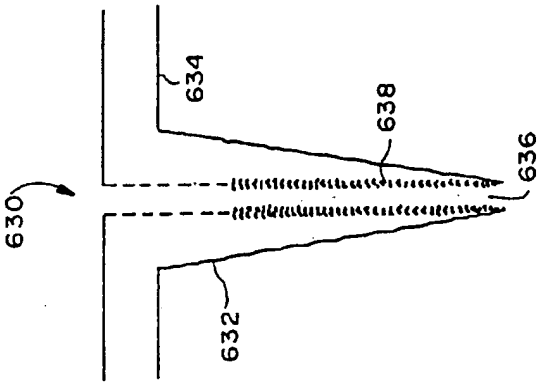


FIG. 27B

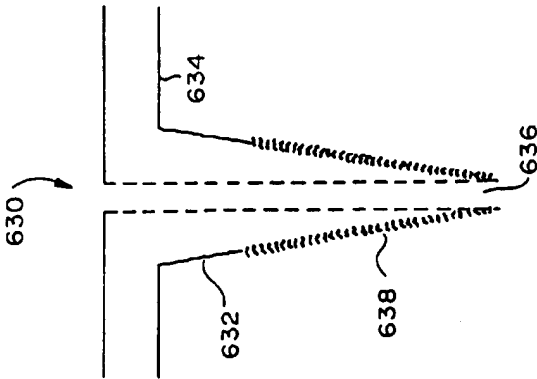


FIG. 27A